

Certificate of Performance
Nitrite Reagent

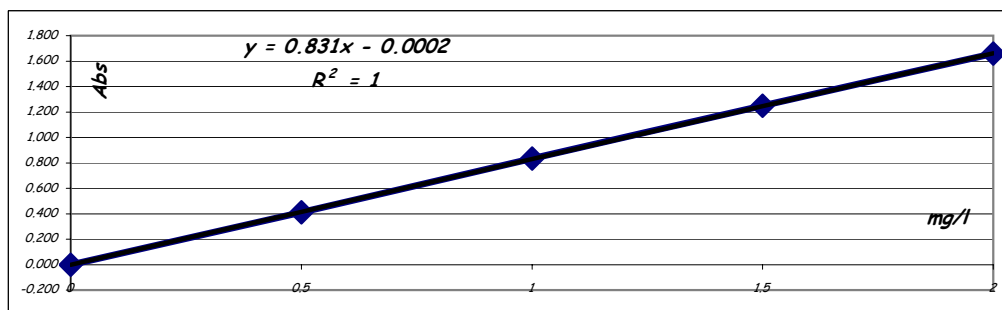
Product Code KR105
Lot Number 6061

Date 16.03.2006

Expiry Date 14.03.2007

Reagent	Lot Number
TON3	6061
Test Method	LTP04
Test Instrument	Konelab 20
Serial Number	P4919028

Standard Value	Lot #	Abs.
0		0.000
0.5	NI0.5 332 05	0.411
1	NI1.0 332 05	0.835
1.5	NI1.5 332 05	1.250
2	NI2.0 332 05	1.658

Calibration Curve


Test	Result	Specification	Pass / Fail
Intercept	0.000	-0.010 to 0.010	Pass
Sensitivity Abs/ppm	0.831	0.750 to 0.900	Pass
Regression	1.000	0.990 to 1.001	Pass

Notes Store between 2 & 8 °C
 *Stable on Board 5 days
 Barcode ID = 105
 * Based on results obtained in our Research Facility



Dr. T. Russell