

'Ready To Use Reagents'



Certificate of Performance

Chloride Reagent


Product Code KR101
Lot Number 6064

Date 20.03.2006 **Expiry Date** 14.03.2007

Reagent	Lot Number
Chloride	6064
Test Method	LTP02
Test Instrument	Konelab 20
Serial Number	P4919028

Standard Value	Lot #	Absorbance
0 ppm		0.005
25 ppm	CL25 332 05	0.309
50 ppm	CL50 332 05	0.572
75 ppm	CL75 332 05	0.788
100 ppm	CL100 332 05	0.956

Calibration Curve

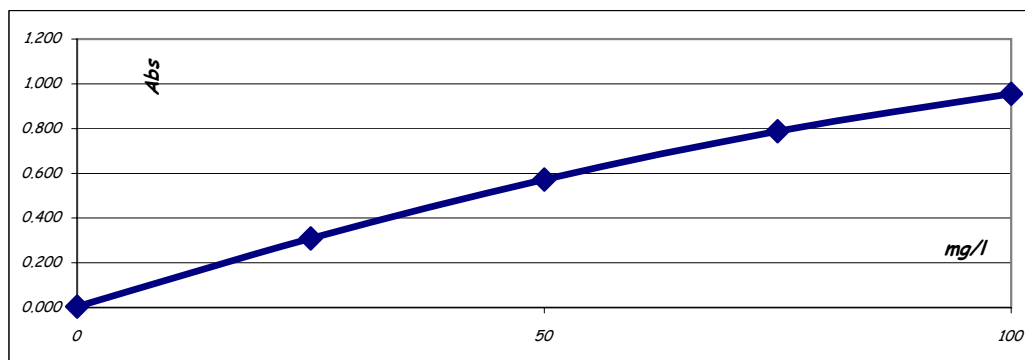

Test	Result	Specification	Pass / Fail
Intercept	0.005	-0.005 to 0.01	Pass
Sensitivity Abs/ppm			
0 - 25 mg/l	0.012	0.0100 to 0.0140	Pass
25 - 50 mg/l	0.011	0.0080 to 0.0120	Pass
50 - 75 mg/l	0.009	0.0065 to 0.0095	Pass
75 - 100 mg/l	0.007	0.0050 to 0.0080	Pass

Notes Store between 2 & 8 °C
 *Stable on Board 5 days
 Barcode ID = 101
 * Based on results obtained in our Research Facility

Tom Russell

Dr. T. Russell