

**Certificate of Performance**

**TON 3 Reagent**

**Product Code** KR 105

**Lot Number** 6074


**Date** 10.04.2006

**Expiry Date** 10.04.2007

Reagent	Lot Number
TON 1	6072
TON 2	6073
<b>TON 3</b>	<b>6074</b>
<b>Test Method</b>	LMTPO3
<b>Test Instrument</b>	Konelab 20
<b>Serial Number</b>	P4919028

Std. Value	Lot #	Abs.
0		0.002
2.5	TON2.5 332 05	0.169
5	TON5.0 332 05	0.329
7.5	TON7.5 332 05	0.480
10	TON10 332 05	0.618

**Calibration Curve**

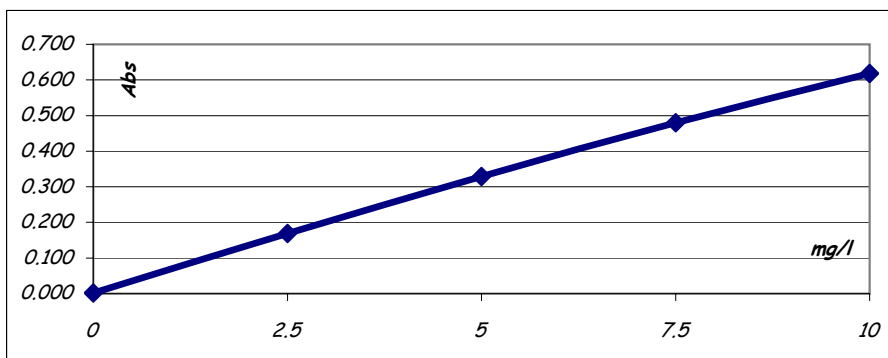

Test	Result	Specification	Pass / Fail
Intercept	0.002	-0.005 to 0.01	<b>Pass</b>
Sensitivity	Abs/ppm		
	0 - 2.5 mg/l	0.0055 to 0.0080	<b>Pass</b>
	2.5 - 5.0 mg/l	0.0060 to 0.0080	<b>Pass</b>
	5.0 - 7.5 mg/l	0.0050 to 0.0075	<b>Pass</b>
	7.5 - 10.0 mg/l	0.0050 to 0.0070	<b>Pass</b>

**Notes** Store between 2 & 8 °c  
 \*Stable on Board 5 days  
 Barcode ID = 105  
 \* Based on results obtained in our Research Facility

*Tom Russell.*

Dr. T. Russell