

'Ready To Use Reagents'



Certificate of Performance

Chloride Reagent


Product Code KR101
Lot Number 6079

Date 14.04.2006 **Expiry Date** 10.04.2007

Reagent	Lot Number
Chloride	6079
Test Method	LTP02
Test Instrument	Konelab 20
Serial Number	P4919028

Standard Value	Lot #	Absorbance
0 ppm		0.005
250 ppm	CL250 090 06	0.319
500 ppm	CL500 090 06	0.520
750 ppm	CL750 090 06	0.669
1000 ppm	CL1000 090 06	0.789

Calibration Curve

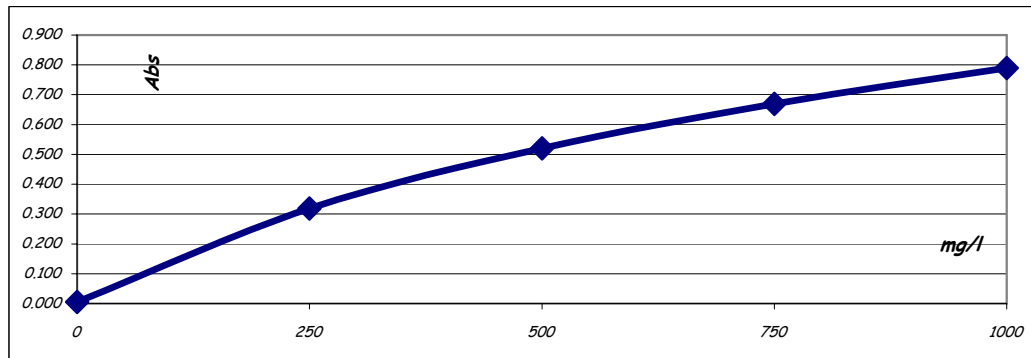

Test	Result	Specification	Pass / Fail
Intercept	0.005	-0.005 to 0.01	Pass
Sensitivity Abs/ppm			
0 - 250 mg/l	0.0013	0.0010 to 0.0016	Pass
250 - 500 mg/l	0.0008	0.0006 to 0.0012	Pass
500 - 750 mg/l	0.0006	0.0004 to 0.0010	Pass
750 - 1000 mg/l	0.0005	0.0003 to 0.0008	Pass

Notes Store between 2 & 8 °c
 *Stable on Board 5 days
 Barcode ID = 101
 * Based on results obtained in our Research Facility

Tom Russell

Dr. T. Russell