

Certificate of Performance

Ammonia 2 Reagent

Product Code KR109
Lot Number 6097


Date 09.06.2006

Expiry Date 01.06.2007

Reagent	Lot Number
AMM 1	6096
AMM 2	6097
Test Method	LTP06
Test Instrument	Konelab 20
Serial Number	P4919028

Std. Value	Lot #	Abs.
0		0.022
0.25	AM0.25 332 05	0.223
0.5	AM0.5 332 05	0.429
0.8	AM0.8 332 05	0.670
1	AM1.0 332 05	0.823

Calibration Curve

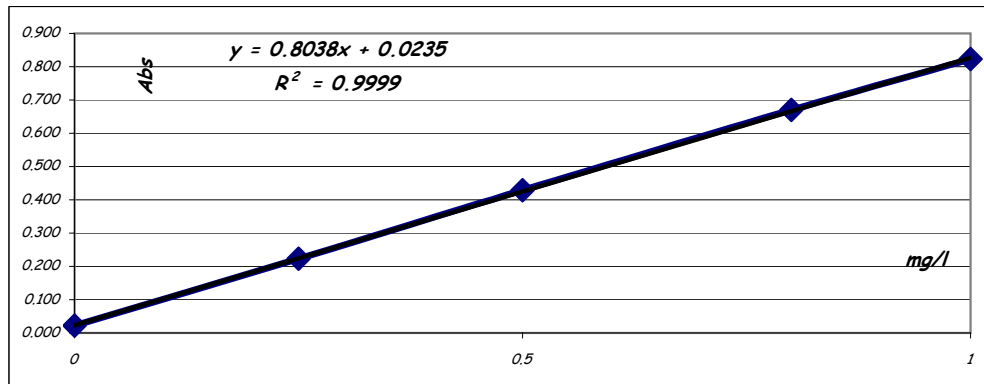

Test	Result	Specification	Pass / Fail
Intercept	0.0235	0.000 to 0.025	Pass
Sensitivity Abs/ppm	0.8036	0.750 to 0.900	Pass
Regression	0.9999	0.990 to 1.0001	Pass

Notes *Store between 2 & 8 °C*

**Stable on Board 5 days*

Barcode ID = 109

** Based on results obtained in our Research Facility*



Dr. T. Russell