

**Certificate of Performance**

**Sulphate Reagent**

**Product Code** KR102  
**Lot Number** 6099


**Date** 12.06.2006

**Expiry Date** 01.06.2007

<b>Reagent</b>	<b>Lot Number</b>
Sulphate	6099
<b>Test Method</b>	LTP01 (1000)
<b>Test Instrument</b>	Konelab 20
<b>Serial Number</b>	P4919028

Standard Value	Lot #	Abs.
0		0.004
250	SU250 332 05	0.092
500	SU500 332 05	0.223
750	SU750 332 05	0.363
1000	SU1000 332 05	0.503

**Calibration Curve**

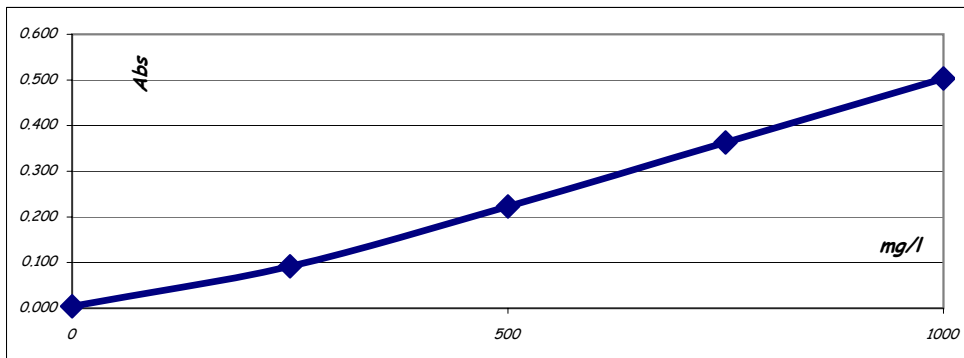

Test	Result	Specification	Pass / Fail
Intercept	0.004	-0.005 to 0.010	<b>Pass</b>
Sensitivity Abs/ppm			
0 - 250 mg/l	0.00037	0.0003 to 0.0005	<b>Pass</b>
250 - 500 mg/l	0.00052	0.0003 to 0.0006	<b>Pass</b>
500 - 750 mg/l	0.00056	0.0004 to 0.0007	<b>Pass</b>
750 - 1000 mg/l	0.00056	0.0004 to 0.0007	<b>Pass</b>

**Notes** Store between 2 & 8 °c  
\*Stable on Board 5 days  
Barcode ID = 102  
\* Based on results obtained in our Research Facility

*Tom Russell*

Dr. T. Russell