

Certificate of Performance

Phosphate 2 (Phos 2) Reagent

Product Code KR107
 Lot Number 6114

Date 11.07.2006


Expiry Date 11.07.2007

Reagent	Lot Number
Phos 1	6113
Phos 2	6114
Test Method	LTP 05
Test Instrument	Konelab 20
Serial Number	P4919028

Standard Value	Lot #	Abs.
0		0.001
0.5	P20 187 06	0.141
1	P20 187 06	0.287
1.5	P20 187 06	0.437
2	P20 187 06	0.566

*serial dilution

Calibration Curve

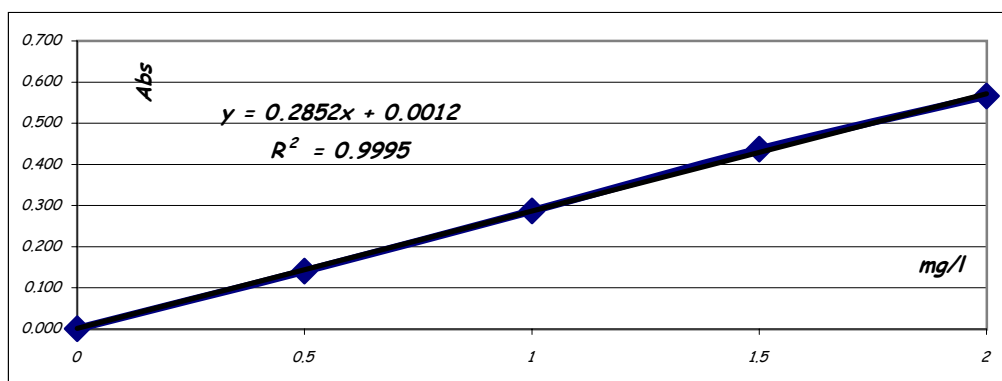

Test	Result	Specification	Pass / Fail
Intercept	0.001	-0.005 to 0.010	Pass
Sensitivity Abs/ppm	0.285	0.260 to 0.320	Pass
Regression	0.999	0.990 to 1.001	Pass

Notes Store between 2 & 8 °C
 *Stable on Board 5 days
 Barcode ID = 106
 * Based on results obtained in our Research Facility

Tom Russell.
 Dr. T. Russell