

**Certificate of Performance**

**TON 3**

Product Code KR105

Date 12.07.2006


Expiry Date 12.07.2007

Reagent	Lot Number
TON 1	6115
TON 2	6117
TON 3	6118
Test Method	LMTPO3
Test Instrument	Konelab 20
Serial Number	P4919028

Std. Value	Lot #	Abs.
0		0.003
2.5	TON 100 187 06	0.178
5	TON 100 187 06	0.337
7.5	TON 100 187 06	0.498
10	TON 100 187 06	0.635

\*serial dilution

**Calibration Curve**

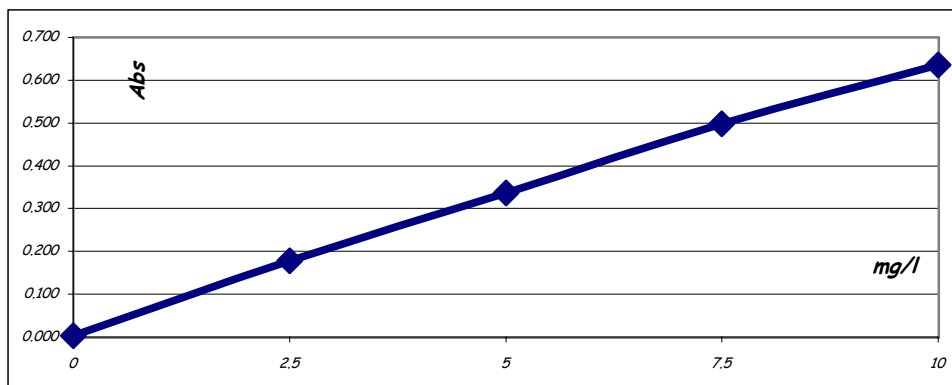

Test	Result	Specification	Pass / Fail
Intercept	0.003	-0.005 to 0.01	Pass
Sensitivity	Abs/ppm		
	0 - 2.5 mg/l	0.0700 to 0.0800	Pass
	2.5 - 5.0 mg/l	0.0636 to 0.0800	Pass
	5.0 - 7.5 mg/l	0.0644 to 0.0800	Pass
	7.5 - 10.0 mg/l	0.0548 to 0.0700	Pass

**Notes** Store between 2 & 8 °C  
 \*Stable on Board TON 1 - 1 day  
 \* TON 2 & TON 3 - 5 days  
 Keep Tightly Sealed when not in use.  
 Do not return unused portions to container  
 Barcode ID- TON 1 103; TON 2 104; TON 3 105  
 \* Based on results obtained in our Research Facility



Dr. T. Russell