

### Certificate of Performance

#### Ammonia 1 Reagent

**Product Code**            **KR108**  
**Lot Number**                **6119**

**Date**            13.07.2006


**Expiry Date**            13.07.2007

Reagent	Lot Number
AMM 1	<b>6119</b>
Amm 2	6120
<b>Test Method</b>	LTP06
<b>Test Instrument</b>	Konelab 20
<b>Serial Number</b>	P4919028

Std. Value	Lot #	Abs.
0.00		0.027
0.25	AMM 10 188 06	0.217
0.50	AMM 10 188 06	0.421
0.77	AMM 10 188 06	0.641
1.00	AMM 10 188 06	0.830

*\*serial dilution*

#### Calibration Curve

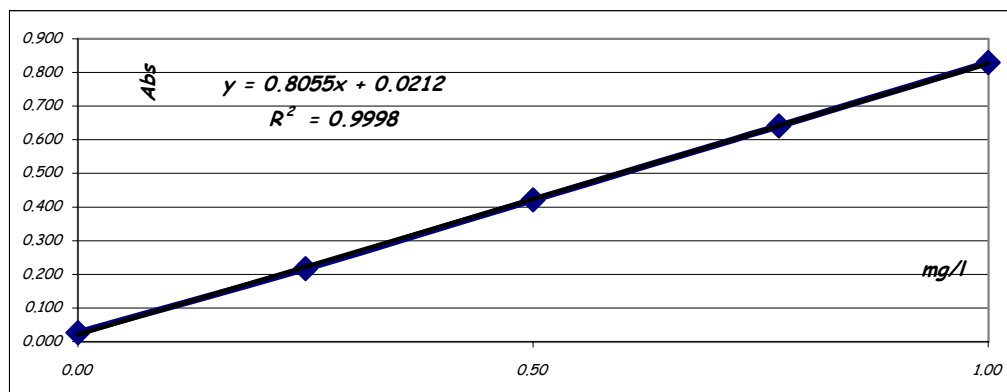

Test	Result	Specification	Pass / Fail
Intercept	0.0212	0.000 to 0.025	<b>Pass</b>
Sensitivity Abs/ppm	0.8055	0.750 to 0.830	<b>Pass</b>
Regression	0.9998	0.990 to 1.0001	<b>Pass</b>

*Notes*    *Store between 2 & 8 ° c*

*\*Stable on Board 1 day*

*Barcode ID = 108*

*\* Based on results obtained in our Research Facility*



*Dr. T. Russell*