

Certificate of Performance

Phosphate 2 (Phos 2) Reagent

Product Code KR107

Lot Number 6146

Date 03.08.2006


Expiry Date 31.07.07

Reagent	Lot Number
Phos 1	6145
Phos 2	6146
Test Method	LTP 05
Test Instrument	Konelab 20
Serial Number	P4919028

Standard Value	Lot #	Abs.
0		0.001
0.5	P20 187 06	0.143
1	P20 187 06	0.287
1.5	P20 187 06	0.437
2	P20 187 06	0.567

*serial dilution

Calibration Curve

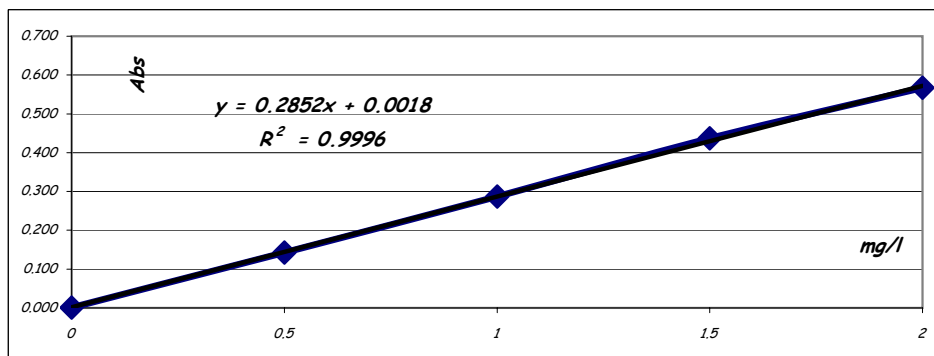

Test	Result	Specification	Pass / Fail
Intercept	0.002	-0.005 to 0.010	Pass
Sensitivity Abs/ppm	0.285	0.260 to 0.320	Pass
Regression	1.000	0.990 to 1.001	Pass

Notes Store between 2 & 8 °C
 *Stable on Board 5 days
 Barcode ID = 106
 * Based on results obtained in our Research Facility

Tom Russell.
 Dr. T. Russell