

Certificate of Performance

Ammonia 2 Reagent

Product Code **KR 109**
Lot Number **6148**

Date 08.08.06


Expiry Date 01.08.07

Reagent	Lot Number
AMM 1	6147
Amm 2	6148
Test Method	LTP06
Test Instrument	Konelab 20
Serial Number	P4919028

Std. Value	Lot #	Abs.
0.00		0.025
0.25	amm 0806	0.226
0.50	amm 0806	0.441
0.77	amm 0806	0.667
1.00	amm 0806	0.857

**serial dilution*

Calibration Curve

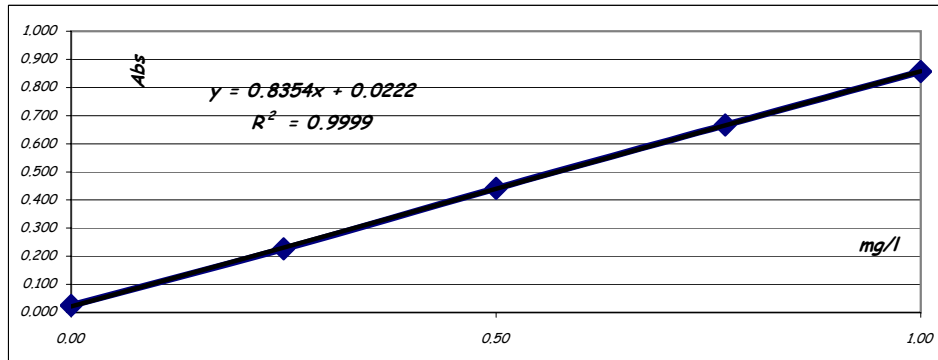

Test	Result	Specification	Pass / Fail
Intercept	0.0222	0.000 to 0.025	Pass
Sensitivity Abs/ppm	0.8354	0.750 to 0.840	Pass
Regression	0.9999	0.990 to 1.0001	Pass

Notes *Store between 2 & 8 °C*
 **Stable on Board 5 days*
 Barcode ID = 109
 ** Based on results obtained in our Research Facility*



Dr. T. Russell