

**Certificate of Performance**

**Chloride Reagent**


**Product Code** KR101  
**Lot Number** 6149

**Date** 08.08.06 **Expiry Date** 28.07.07

Reagent	Lot Number
Chloride	6149
Test Method	LTP02
Test Instrument	Konelab 20
Serial Number	P4919028

Standard Value	Lot #	Absorbance
0 ppm		0.004
250 ppm	CL 4000 07 06	0.305
500 ppm	CL 4000 07 06	0.493
800 ppm	CL 4000 07 06	0.647
1000 ppm	CL 4000 07 06	0.728

**Calibration Curve**

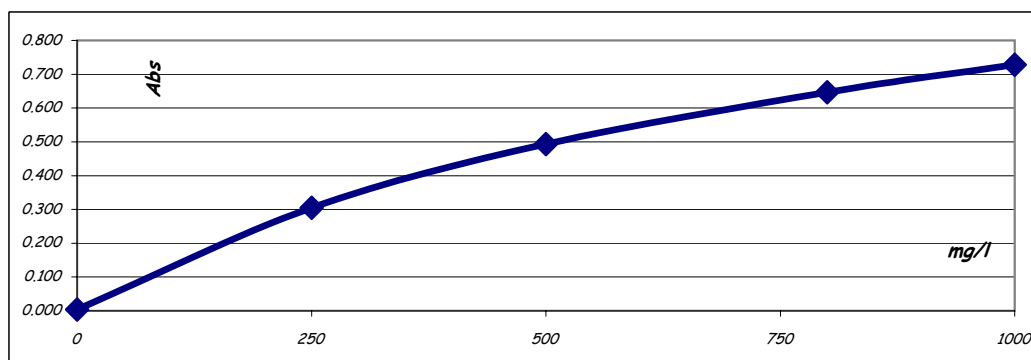

Test	Result	Specification	Pass / Fail
Intercept	0.004	-0.005 to 0.01	Pass
Sensitivity Abs/ppm			
0 - 250 mg/l	0.0012	0.0010 to 0.0016	Pass
250 - 500 mg/l	0.0008	0.0006 to 0.0012	Pass
500 - 800 mg/l	0.0005	0.0004 to 0.0010	Pass
800 - 1000 mg/l	0.0004	0.0003 to 0.0008	Pass

**Notes** Store between 2 & 8 °C  
 \*Stable on Board 5 days  
 Barcode ID = 101  
 \*Based on results obtained in our Research Facility



Dr. T. Russell