

Certificate of Performance

Ammonia 2 Reagent

Product Code **KR 109**
Lot Number **6167**

Date 07.09.06


Expiry Date 06.09.07

Reagent	Lot Number
AMM 1	6166
Amm 2	6167
Test Method	LTP06
Test Instrument	Konelab 20
Serial Number	P4919028

Std. Value	Lot #	Abs.
0.00		0.020
0.25	Amm 10 0806	0.219
0.50	Amm 10 0806	0.428
0.77	Amm 10 0806	0.653
1.00	Amm 10 0806	0.847

**serial dilution*

Calibration Curve

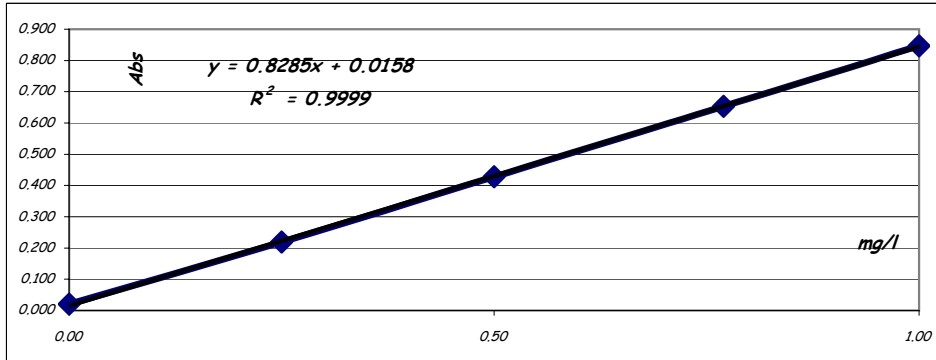

Test	Result	Specification	Pass / Fail
Intercept	0.0158	0.000 to 0.025	Pass
Sensitivity Abs/ppm	0.8285	0.750 to 0.830	Pass
Regression	0.9999	0.990 to 1.0001	Pass

Notes *Store between 2 & 8 °C*

**Stable on Board 5 days*

Barcode ID = 109

** Based on results obtained in our Research Facility*



Dr. T. Russell