

Certificate of Performance

TON 2

Product Code KR104

Date 01.10.2006


Expiry Date 01.10.2007

Reagent	Lot Number
TON 1	6173
TON 2	6174
TON 3	6175
Test Method	LMTPO3
Test Instrument	Konelab 20
Serial Number	P4919028

Std. Value	Lot #	Abs.
0.00		0.002
2.50	TON 10 08 06	0.196
5.00	TON 10 08 06	0.365
7.69	TON 10 08 06	0.514
10.00	TON 10 08 06	0.643

*serial dilution

Calibration Curve

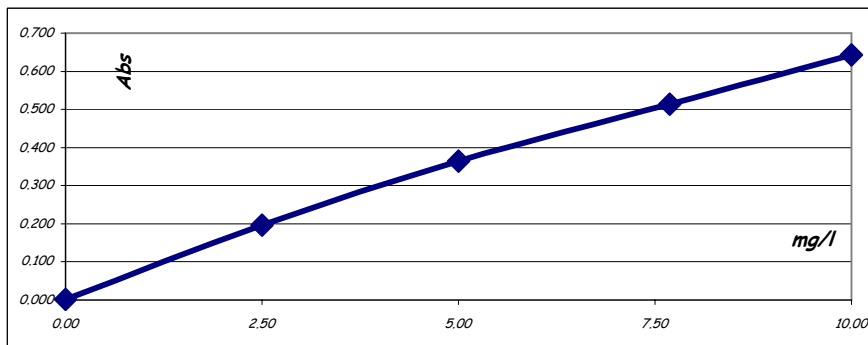

Test	Result	Specification	Pass / Fail
Intercept	0.002	-0.005 to 0.01	Pass
Sensitivity Abs/ppm			
0 - 2.50 mg/l	0.0776	0.0550 to 0.0800	Pass
2.50 - 5.00 mg/l	0.0676	0.0600 to 0.0800	Pass
5.00 - 7.69 mg/l	0.0554	0.0550 to 0.0800	Pass
7.69 - 10.0 mg/l	0.0558	0.0500 to 0.0700	Pass

Notes Store between 2 & 8 °C
 *Stable on Board TON 1 - 1 day
 * TON 2 & TON 3 - 5 days:
 Keep Tightly Sealed when not in use.
 Do not return unused portions to container
 Barcode ID- TON 1 103; TON 2 104; TON 3 105
 * Based on results obtained in our Research Facility



Dr. T. Russell