

### Certificate of Performance

#### Ammonia 1 Reagent

**Product Code**      **KR108**  
**Lot Number**        **6179**

**Date**      01.10.2006


**Expiry Date**      01.10.2007

Reagent	Lot Number
AMM 1	<b>6179</b>
Amm 2	6178
<b>Test Method</b>	LTP06
<b>Test Instrument</b>	Konelab 20
<b>Serial Number</b>	P4919028

Std. Value	Lot #	Abs.
0.00		0.012
0.25	AMM 10 0806	0.214
0.50	AMM 10 0806	0.428
0.77	AMM 10 0806	0.653
1.00	AMM 10 0806	0.838

*\*serial dilution*

#### Calibration Curve

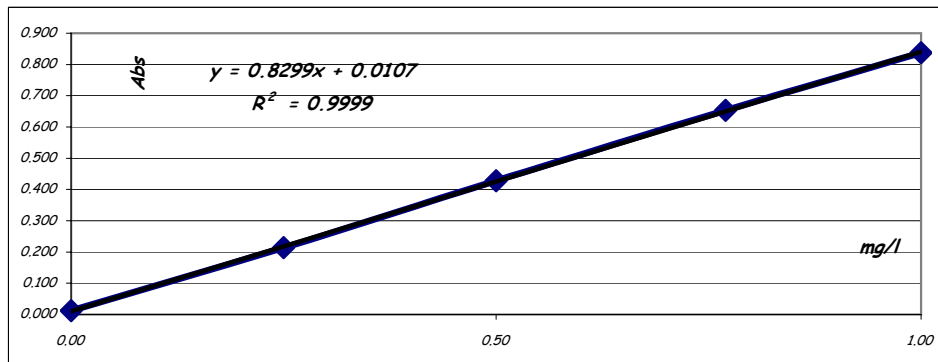

Test	Result	Specification	Pass / Fail
Intercept	0.0107	0.000 to 0.025	<b>Pass</b>
Sensitivity Abs/ppm	0.8299	0.750 to 0.830	<b>Pass</b>
Regression	0.9999	0.990 to 1.0001	<b>Pass</b>

**Notes**      *Store between 2 & 8 °C*  
                  *\*Stable on Board 1 day*  
                  *Barcode ID = 108*  
                  *\* Based on results obtained in our Research Facility*


---

*Dr. T. Russell*