

Certificate of Performance

Ammonia 2 Reagent

Product Code **KR 109**
Lot Number **6190**

Date 10.11.2006


Expiry Date 10.11.2007

Reagent	Lot Number
AMM 1	6189
Amm 2	6190
Test Method	LTP06
Test Instrument	Konelab 20
Serial Number	P4919028

Std. Value	Lot #	Abs.
0.00		0.020
0.25	Amm 10 0806	0.213
0.50	Amm 10 0806	0.415
0.77	Amm 10 0806	0.632
1.00	Amm 10 0806	0.824

**serial dilution*

Calibration Curve

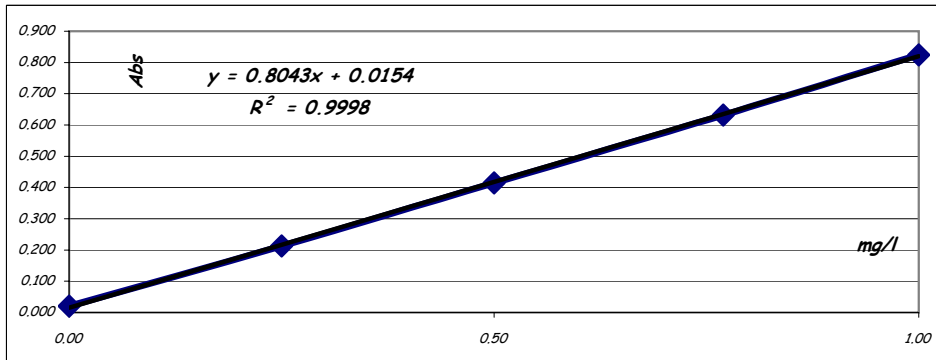

Test	Result	Specification	Pass / Fail
Intercept	0.0154	0.000 to 0.025	Pass
Sensitivity Abs/ppm	0.8043	0.750 to 0.830	Pass
Regression	0.9998	0.990 to 1.0001	Pass

Notes *Store between 2 & 8 °C*
 **Stable on Board 5 days*
 Barcode ID = 109
 ** Based on results obtained in our Research Facility*



Dr. T. Russell