

Certificate of Performance

Nitrite Reagent

Product Code **KR105**
Lot Number **6192**

Date 13.11.2006


Expiry Date 13.11.2007

Reagent	Lot Number
TON3	6192
Test Method	LTP04
Test Instrument	Konelab 20
Serial Number	P4919028

Standard Value	Lot #	Abs.
0		0.001
0.50	NO2-20 08 06	0.413
1.00	NO2-20 08 06	0.809
1.54	NO2-20 08 06	1.240
2.00	NO2-20 08 06	1.631

*serial dilution

Calibration Curve

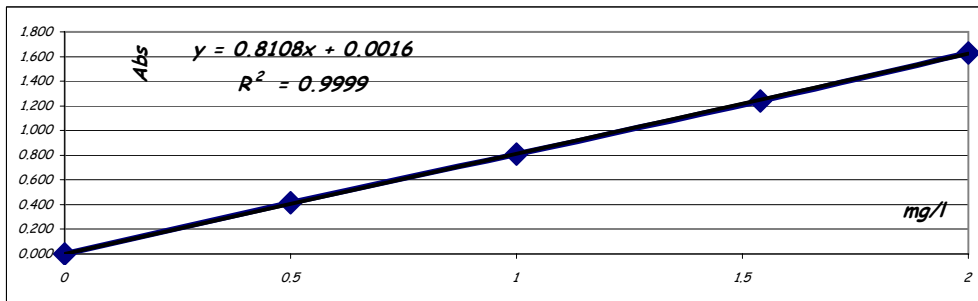

Test	Result	Specification	Pass / Fail
Intercept	0.002	-0.010 to 0.010	Pass
Sensitivity Abs/ppm	0.811	0.750 to 0.900	Pass
Regression	1.000	0.990 to 1.001	Pass

Notes *Store between 2 & 8 °C*
**Stable on Board 5 days*
Barcode ID = 105
** Based on results obtained in our Research Facility*



Dr. T. Russell