

Certificate of Performance

TON 3

Product Code KR105

Date 13.11.2006


Expiry Date 13.11.2007

Reagent	Lot Number
TON 1	6168
TON 2	6191
TON 3	6192
Test Method	LMTP03
Test Instrument	Konelab 20
Serial Number	P4919028

Std. Value	Lot #	Abs.
0.00		0.003
2.50	TON 100 08 06	0.178
5.00	TON 100 08 06	0.343
7.69	TON 100 08 06	0.497
10.00	TON 100 08 06	0.624

*serial dilution

Calibration Curve

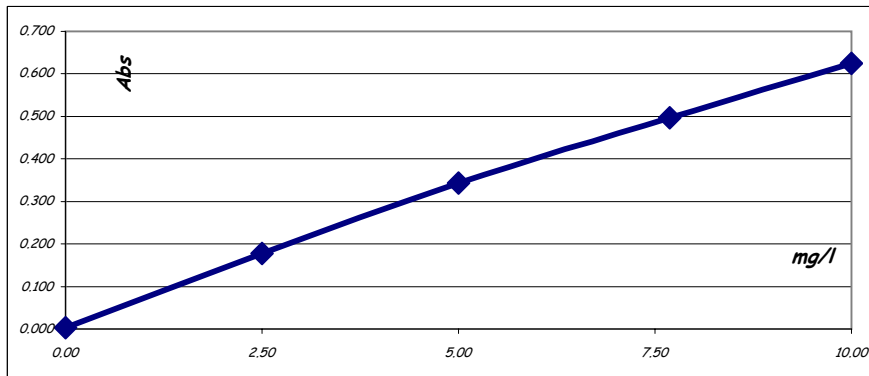

Test	Result	Specification	Pass / Fail
Intercept	0.003	-0.005 to 0.01	Pass
Sensitivity Abs/ppm			
0 - 2.50 mg/l	0.0700	0.0550 to 0.0800	Pass
2.50 - 5.00 mg/l	0.0660	0.0600 to 0.0800	Pass
5.00 - 7.69 mg/l	0.0572	0.0550 to 0.0800	Pass
7.69 - 10.0 mg/l	0.0550	0.0500 to 0.0700	Pass

Notes

- Store between 2 & 8 °C
- *Stable on Board TON 1 - 1 day
- * TON 2 & TON 3 - 5 day:
- Keep Tightly Sealed when not in use.
- Do not return unused portions to container
- Barcode ID- TON 1 103; TON 2 104; TON 3 105
- * Based on results obtained in our Research Facility



Dr. T. Russell