

**Certificate of Performance**

**Chloride Reagent**


**Product Code** KR101  
**Lot Number** 6194

**Date** 15.11.06 **Expiry Date** 15.11.07

Reagent	Lot Number
Chloride	6194
Test Method	LTP02
Test Instrument	Konelab 20
Serial Number	P4919028

Standard Value	Lot #	Absorbance
0 ppm		0.005
250 ppm	CL25009006	0.322
500 ppm	CL50009006	0.522
800 ppm	CL75009006	0.688
1000 ppm	CL100009006	0.778

**Calibration Curve**

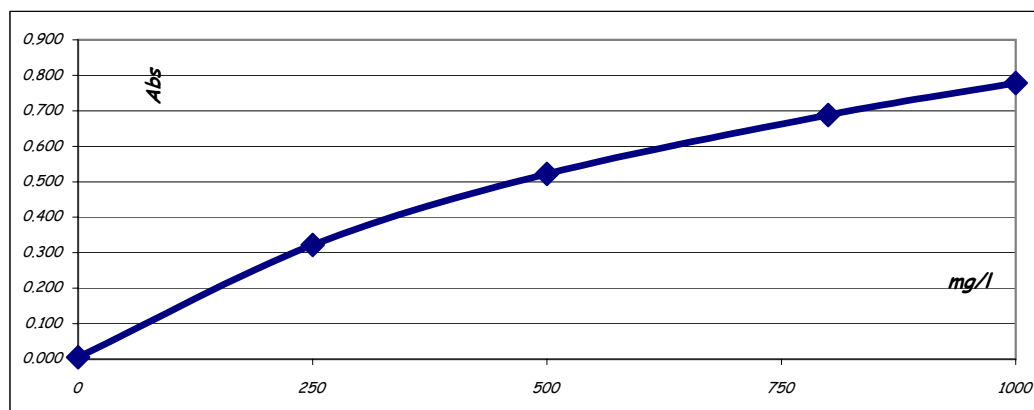

Test	Result	Specification	Pass / Fail
Intercept	0.005	-0.005 to 0.01	<b>Pass</b>
Sensitivity Abs/ppm			
0 - 250 mg/l	0.0013	0.0010 to 0.0016	<b>Pass</b>
250 - 500 mg/l	0.0008	0.0006 to 0.0012	<b>Pass</b>
500 - 800 mg/l	0.0006	0.0004 to 0.0010	<b>Pass</b>
800 - 1000 mg/l	0.0005	0.0003 to 0.0008	<b>Pass</b>

**Notes** Store between 2 & 8 °C  
 \*Stable on Board 5 days  
 Barcode ID = 101  
 \* Based on results obtained in our Research Facility

*Tom Russell*  
 \_\_\_\_\_  
 Dr. T. Russell