Precision®

Labmedics ANALYTICAL SOLUTIONS

*'Ready To Use Reagents'* Ver 2006:03

# Certificate of Performance

## TON 1

Product Code KR103

**Date** 1.12.06 **Expiry Date** 1.12.07

| Reagent | Lot Number |
|---|---|
| **TON 1** | **6199** |
| **TON 2** | 6200 |
| **TON 3** | 6201 |
| **Test Method** | LMTP03 |
| **Test Instrument** | Konelab 20 |
| **Serial Number** | P4919028 |

| Std. Value | Lot # | Abs. |
|---|---|---|
| 0.00 | | 0.003 |
| 2.50 | TON 10 08 06 | 0.177 |
| 5.00 | TON 10 08 06 | 0.343 |
| 7.69 | TON 10 08 06 | 0.505 |
| 10.00 | TON 10 08 06 | 0.633 |

*serial dilution

### Calibration Curve

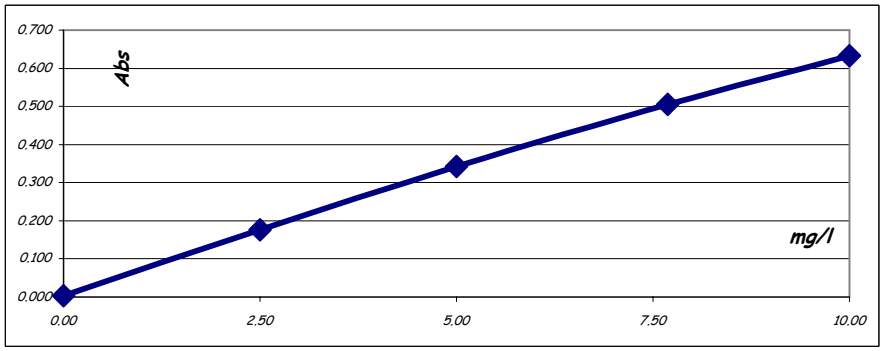


| Test | | Result | Specification | | | Pass / Fail |
|---|---|---|---|---|---|---|
| Intercept | | 0.003 | -0.005 | to | 0.01 | **Pass** |
| Sensitivity | Abs/ppm | | | | | |
| | *0 - 2.50 mg/l* | 0.0696 | 0.0550 | to | 0.0800 | **Pass** |
| | *2.50 - 5.00 mg/l* | 0.0664 | 0.0600 | to | 0.0800 | **Pass** |
| | *5.00 - 7.69 mg/l* | 0.0602 | 0.0550 | to | 0.0800 | **Pass** |
| | *7.69 - 10.0 mg/l* | 0.0554 | 0.0500 | to | 0.0700 | **Pass** |

*Notes* *Store between 2 & 8 °C*

**Stable on Board TON 1 - 1 day*

** TON 2 & TON 3 - 5 days*

*Keep Tightly Sealed when not in use.*

*Do not return unused portions to container*

*Barcode ID- TON 1 103; TON 2 104; TON 3 105*

** Based on results obtained in our Research Facility*

Tom Russell.

*Dr. T. Russell*

Labmedics ANALYTICAL SOLUTIONS

Telegraphic House, Waterfront Quay, Salford Quays, Manchester M50 3XW

Telephone 0161 869 0420