

Certificate of Performance

TON 2

Product Code KR104

Date 1.12.2006


Expiry Date 1.12.2007

Reagent	Lot Number
TON 1	6199
TON 2	6200
TON 3	6201
Test Method	LMTP03
Test Instrument	Konelab 20
Serial Number	P4919028

Std. Value	Lot #	Abs.
0.00		0.003
2.50	TON 10 08 06	0.177
5.00	TON 10 08 06	0.343
7.69	TON 10 08 06	0.505
10.00	TON 10 08 06	0.633

*serial dilution

Calibration Curve

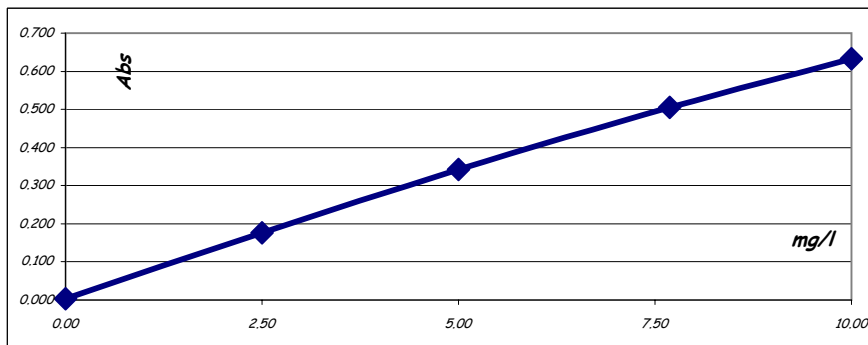

Test	Result	Specification	Pass / Fail
Intercept	0.003	-0.005 to 0.01	Pass
Sensitivity Abs/ppm			
0 - 2.50 mg/l	0.0696	0.0550 to 0.0800	Pass
2.50 - 5.00 mg/l	0.0664	0.0600 to 0.0800	Pass
5.00 - 7.69 mg/l	0.0602	0.0550 to 0.0800	Pass
7.69 - 10.0 mg/l	0.0554	0.0500 to 0.0700	Pass

Notes

- Store between 2 & 8 °C
- *Stable on Board TON 1 - 1 day
- * TON 2 & TON 3 - 5 days:
- Keep Tightly Sealed when not in use.
- Do not return unused portions to container
- Barcode ID- TON 1 103; TON 2 104; TON 3 105
- * Based on results obtained in our Research Facility



Dr. T. Russell