

Certificate of Performance
Phosphate 1 (Phos 1) Reagent
Product Code KR106

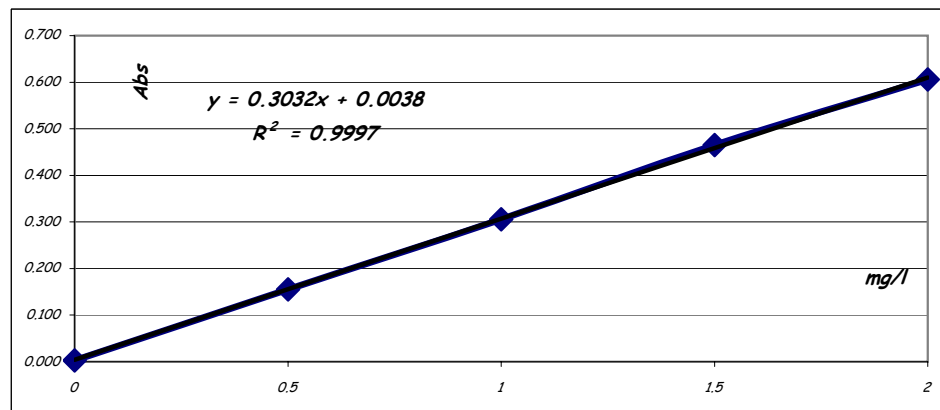
Lot Number 6202

Date 1.12.2006

Expiry Date 1.12.2007

Reagent	Lot Number
Phos 1	6202
Phos 2	6108
Test Method	LTP 05
Test Instrument	Konelab 20
Serial Number	P4919028

Standard Value	Lot #	Abs.
0		0.003
0.5	P20 08 06	0.155
1	P20 08 06	0.306
1.5	P20 08 06	0.465
2	P20 08 06	0.606

**serial dilution*
Calibration Curve


	Result	Specification	Pass / Fail
Intercept	0.004	-0.005 to 0.010	Pass
Sensitivity Abs/ppm	0.303	0.260 to 0.320	Pass
Regression	1.000	0.990 to 1.001	Pass

Notes Store between 2 & 8 °C
 *Stable on Board 5 days
 Barcode ID = 106
 * Based on results obtained in our Research Facility



Dr. T. Russell