

Certificate of Performance

Ammonia 1 Reagent

Product Code **KR108**
Lot Number **6206**

Date 6.12.2006


Expiry Date 6.12.2007

Reagent	Lot Number
AMM 1	6206
Amm 2	6110
Test Method	LTP06
Test Instrument	Konelab 20
Serial Number	P4919028

Std. Value	Lot #	Abs.
0.00		0.016
0.25	AMM 10 0806	0.213
0.50	AMM 10 0806	0.422
0.77	AMM 10 0806	0.630
1.00	AMM 10 0806	0.815

**serial dilution*

Calibration Curve

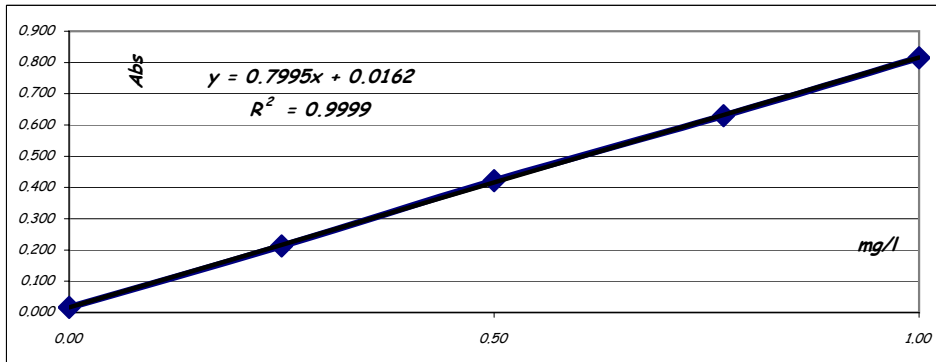

Test	Result	Specification	Pass / Fail
Intercept	0.0162	0.000 to 0.025	Pass
Sensitivity Abs/ppm	0.7995	0.750 to 0.830	Pass
Regression	0.9999	0.990 to 1.0001	Pass

Notes *Store between 2 & 8 °C*

**Stable on Board 1 day*

Barcode ID = 108

** Based on results obtained in our Research Facility*



Dr. T. Russell