

Certificate of Performance

Ammonia 2 Reagent

Product Code **KR 109**
Lot Number **7037**

Date 16.02.2007


Expiry Date 16.02.2008

Reagent	Lot Number
AMM 1	7036
Amm 2	7037
Test Method	LTP06
Test Instrument	Konelab 20
Serial Number	P4919028

Std. Value	Lot #	Abs.
0.00		0.021
0.25	Amm 10 02 07	0.241
0.50	Amm 10 02 07	0.466
0.77	Amm 10 02 07	0.703
1.00	Amm 10 02 07	0.904

**serial dilution*

Calibration Curve

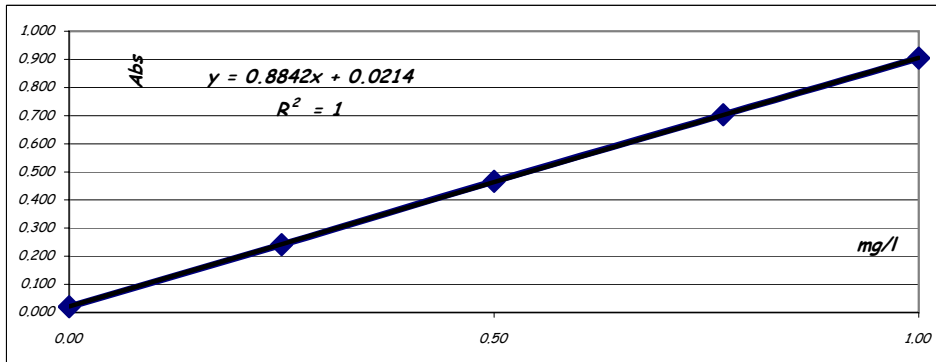

Test	Result	Specification	Pass / Fail
Intercept	0.0214	0.000 to 0.025	Pass
Sensitivity Abs/ppm	0.8842	0.750 to 0.890	Pass
Regression	1.0000	0.990 to 1.0001	Pass

Notes *Store between 2 & 8 °C*
 **Stable on Board 5 days*
 Barcode ID = 109
 ** Based on results obtained in our Research Facility*



Dr. T. Russell