

### Certificate of Performance

#### Nitrite Reagent

**Product Code** KR110  
**Lot Number** 7040

**Date** 16.02.2007


**Expiry Date** 16.02.2008

<b>Reagent</b>	<b>Lot Number</b>
TON 4	7040
<b>Test Method</b>	LTP04
<b>Test Instrument</b>	Konelab 20
<b>Serial Number</b>	P4919028

Standard Value	Lot #	Abs.
0		0.001
0.50	NO2-20 08 06	0.417
1.00	NO2-20 08 06	0.837
1.54	NO2-20 08 06	1.296
2.00	NO2-20 08 06	1.697

\*serial dilution

#### Calibration Curve

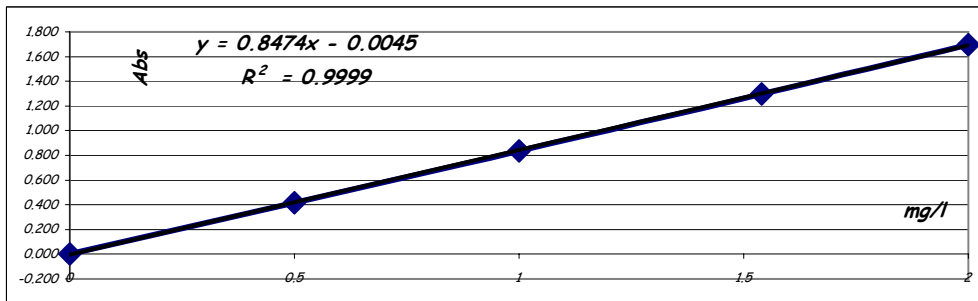

Test	Result	Specification	Pass / Fail
Intercept	-0.005	-0.010 to 0.010	Pass
Sensitivity Abs/ppm	0.847	0.750 to 0.900	Pass
Regression	1.000	0.990 to 1.001	Pass

**Notes** Store between 2 & 8 °C  
 \*Stable on Board 5 days  
 Barcode ID = 110  
 \* Based on results obtained in our Research Facility

*Tom Russell.*  
 Dr. T. Russell