

Certificate of Performance

Chloride Reagent


Product Code KR101
Lot Number 7065

Date 02.04.2007 **Expiry Date** 02.04.2008

Reagent	Lot Number
Chloride	7065
Test Method	LTP02
Test Instrument	Konelab 20
Serial Number	P4919028

Standard Value	Lot #	Absorbance
0 ppm		0.005
250 ppm	CL25009006	0.320
500 ppm	CL50009006	0.511
800 ppm	CL75009006	0.665
1000 ppm	CL100009006	0.752

Calibration Curve

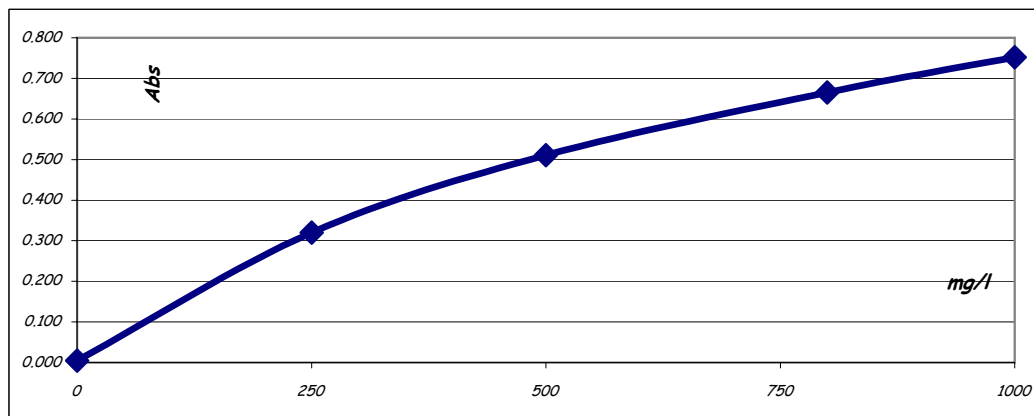

Test	Result	Specification	Pass / Fail
Intercept	0.005	-0.005 to 0.01	Pass
Sensitivity Abs/ppm			
0 - 250 mg/l	0.0013	0.0010 to 0.0016	Pass
250 - 500 mg/l	0.0008	0.0006 to 0.0012	Pass
500 - 800 mg/l	0.0005	0.0004 to 0.0010	Pass
800 - 1000 mg/l	0.0004	0.0003 to 0.0008	Pass

Notes Store between 2 & 8 °C
 *Stable on Board 5 days
 Barcode ID = 101
 *Based on results obtained in our Research Facility

Tom Russell

Dr. T. Russell