

## Certificate of Performance

### TON 2

Product Code KR104

**Date** 06.07.2007


**Expiry Date** 09.07.2008

Reagent	Lot Number
TON 1	7146
TON 2	<b>7147</b>
TON 3	7148
<b>Test Method</b>	LMTPO3
<b>Test Instrument</b>	Konelab 20
<b>Serial Number</b>	P4919028

Std. Value	Lot #	Abs.
0.00		0.005
2.50	TON 100 02 07	0.178
5.00	TON 100 02 07	0.343
7.69	TON 100 02 07	0.507
10.00	TON 100 02 07	0.630

\*serial dilution

### Calibration Curve

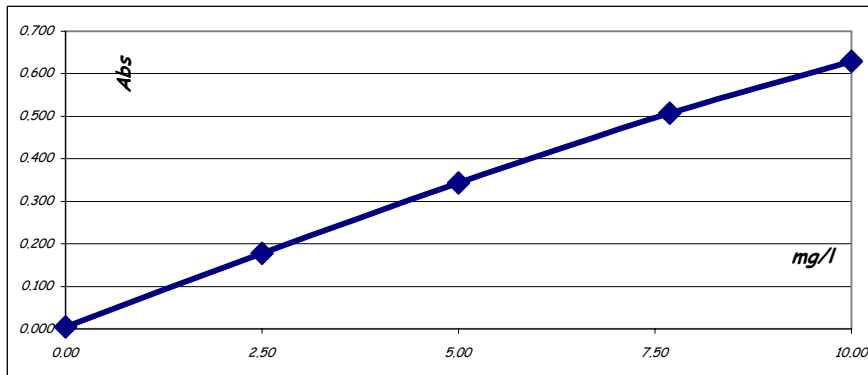

Test	Result	Specification	Pass / Fail
Intercept	0.005	-0.005 to 0.01	<b>Pass</b>
Sensitivity Abs/ppm			
0 - 2.50 mg/l	0.0692	0.0550 to 0.0800	<b>Pass</b>
2.50 - 5.00 mg/l	0.0660	0.0600 to 0.0800	<b>Pass</b>
5.00 - 7.69 mg/l	0.0610	0.0550 to 0.0800	<b>Pass</b>
7.69 - 10.0 mg/l	0.0532	0.0500 to 0.0700	<b>Pass</b>

**Notes** Store between 2 & 8 °C  
 \*Stable on Board TON 1 - 1 day  
                   \* TON 2 & TON 3 - 5 day:  
 Keep Tightly Sealed when not in use.  
 Do not return unused portions to container  
 Barcode ID- TON 1 103; TON 2 104; TON 3 105  
 \* Based on results obtained in our Research Facility



Dr. T. Russell