

### Certificate of Performance

#### Ammonia 2 Reagent

**Product Code**      **KR 109**  
**Lot Number**        **7189**

**Date**      29.08.2007


**Expiry Date**      27.08.2008

<b>Reagent</b>	<b>Lot Number</b>
AMM 1	7188
Amm 2	<b>7189</b>
<b>Test Method</b>	LTP06
<b>Test Instrument</b>	Konelab 20
<b>Serial Number</b>	P4919028

<b>Std. Value</b>	<b>Lot #</b>	<b>Abs.</b>
0.00		0.017
0.25	Amm 10 08 07	0.217
0.50	Amm 10 08 07	0.421
0.77	Amm 10 08 07	0.641
1.00	Amm 10 08 07	0.838

*\*serial dilution*

#### Calibration Curve

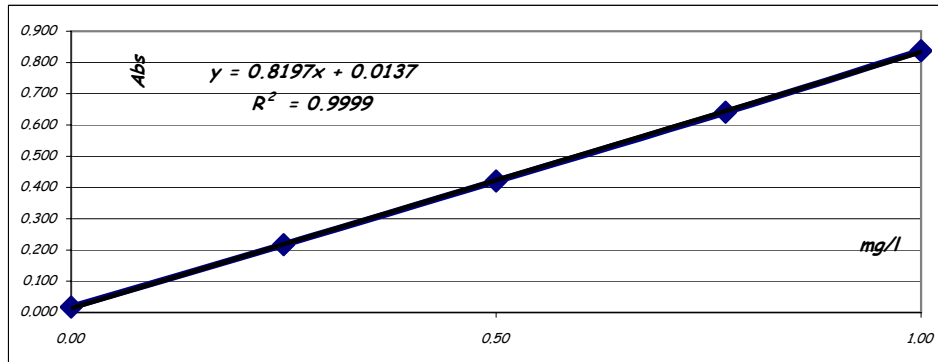

Test	Result	Specification	Pass / Fail
Intercept	0.0137	0.000 to 0.025	<b>Pass</b>
Sensitivity Abs/ppm	0.8197	0.750 to 0.890	<b>Pass</b>
Regression	0.9999	0.990 to 1.0001	<b>Pass</b>

**Notes**      *Store between 2 & 8 °C*  
                  *\*Stable on Board 5 days*  
                  *Barcode ID = 109*  
                  *\* Based on results obtained in our Research Facility*


---

*Dr. T. Russell*