

**Certificate of Performance**
**Phosphate 2 (Phos 2) Reagent**
**Product Code** KR107

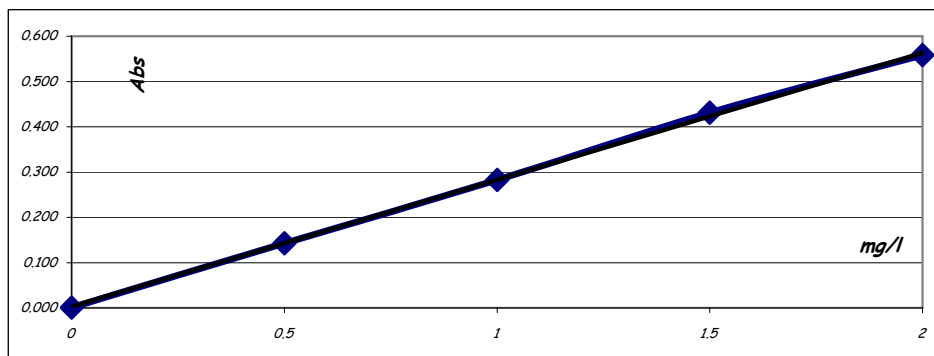
**Lot Number** 7199

**Date** 21.09.2007

**Expiry Date** 14.09.2008

Reagent	Lot Number
Phos 1	7045
Phos 2	7199
<b>Test Method</b>	LTP 05
<b>Test Instrument</b>	Konelab 20
<b>Serial Number</b>	P4919028

Standard Value	Lot #	Abs.
0		0.001
0.5	P20 08 07	0.143
1	P20 08 07	0.283
1.5	P20 08 07	0.431
2	P20 08 07	0.558

*\*serial dilution*
**Calibration Curve**


Test	Result	Specification	Pass / Fail
Intercept	0.003	-0.005 to 0.010	<b>Pass</b>
Sensitivity Abs/ppm	0.280	0.260 to 0.320	<b>Pass</b>
Regression	1.000	0.990 to 1.001	<b>Pass</b>

Notes Store between 2 & 8 °C  
 \*Stable on Board 5 days  
 Barcode ID = 107  
 \* Based on results obtained in our Research Facility

  
 Dr. T. Russell