

### Certificate of Performance

#### Ammonia 2 Reagent

**Product Code**      **KR 109**  
**Lot Number**        **7225**

**Date**      18.10.2007


**Expiry Date**      10.10.2008

Reagent	Lot Number
AMM 1	7194
Amm 2	7225
<b>Test Method</b>	LTP06
<b>Test Instrument</b>	Konelab 20
<b>Serial Number</b>	P4919028

Std. Value	Lot #	Abs.
0.00		0.014
0.25	Amm 10 08 07	0.229
0.50	Amm 10 08 07	0.448
0.77	Amm 10 08 07	0.683
1.00	Amm 10 08 07	0.885

*\*serial dilution*

#### Calibration Curve

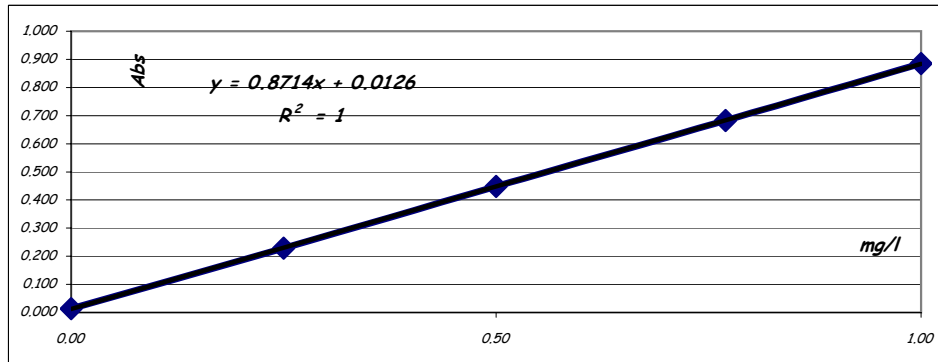

Test	Result	Specification	Pass / Fail
Intercept	0.0126	0.000 to 0.025	<b>Pass</b>
Sensitivity Abs/ppm	0.8714	0.750 to 0.890	<b>Pass</b>
Regression	1.0000	0.990 to 1.0001	<b>Pass</b>

**Notes**      *Store between 2 & 8 °C*  
                   *\*Stable on Board 5 days*  
                   *Barcode ID = 109*  
                   *\* Based on results obtained in our Research Facility*


---

*Dr. T. Russell*