

Certificate of Performance

Ammonia 1 Reagent

Product Code **KR108**
Lot Number **7235**

Date 09.11.2007


Expiry Date 01.11.2008

| Reagent | Lot Number |
|------------------------|-------------|
| AMM 1 | 7235 |
| Amm 2 | 7207 |
| Test Method | LTP06 |
| Test Instrument | Konelab 20 |
| Serial Number | P4919028 |

| Std. Value | Lot # | Abs. |
|------------|--------------|-------|
| 0.00 | | 0.022 |
| 0.25 | AMM 10 08 07 | 0.215 |
| 0.50 | AMM 10 08 07 | 0.419 |
| 0.77 | AMM 10 08 07 | 0.646 |
| 1.00 | AMM 10 08 07 | 0.830 |

**serial dilution*

Calibration Curve

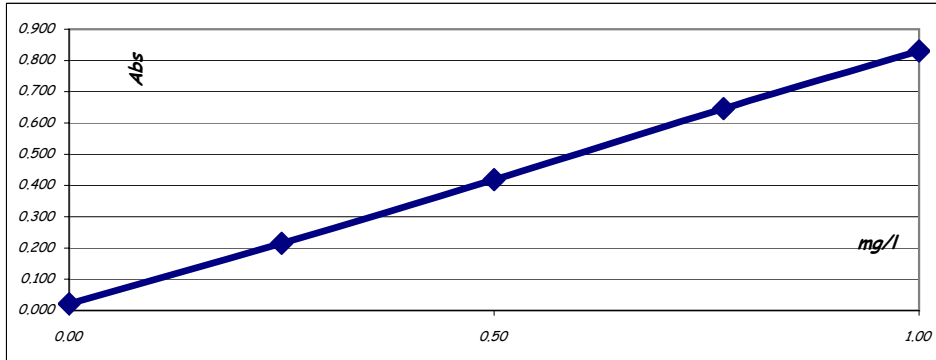

| Test | Result | Specification | Pass / Fail |
|---------------------|--------|-----------------|-------------|
| Intercept | 0.0169 | 0.000 to 0.025 | Pass |
| Sensitivity Abs/ppm | 0.8124 | 0.750 to 0.890 | Pass |
| Regression | 0.9998 | 0.990 to 1.0001 | Pass |

Notes *Store between 2 & 8 °C*

**Stable on Board 1 day*

Barcode ID = 108

** Based on results obtained in our Research Facility*



Dr. T. Russell