

Certificate of Performance

Nitrite Reagent

Product Code KR105
Lot Number 7253

Date 21.11.2007


Expiry Date 19.11.2008

Reagent	Lot Number
TON3	7253
Test Method	LTP04
Test Instrument	Konelab 20
Serial Number	P4919028

Standard Value	Lot #	Abs.
0		0.001
0.50	NO2-20 11 07	0.451
1.00	NO2-20 11 07	0.877
1.54	NO2-20 11 07	1.332
2.00	NO2-20 11 07	1.734

*serial dilution

Calibration Curve

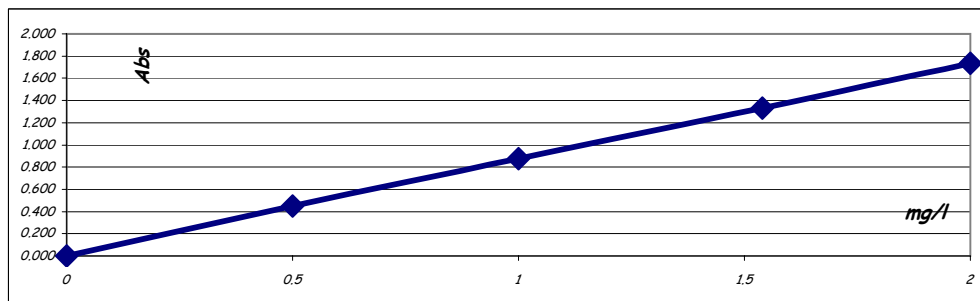

Test	Result	Specification	Pass / Fail
Intercept	0.010	-0.010 to 0.010	Pass
Sensitivity Abs/ppm	0.862	0.750 to 0.900	Pass
Regression	1.000	0.990 to 1.001	Pass

Notes Store between 2 & 8 °C
 *Stable on Board 5 days
 Barcode ID = 105
 * Based on results obtained in our Research Facility

Tom Russell.
 Dr. T. Russell