

Certificate of Performance

**Phosphate 2 (Phos 2) Reagent**

**Product Code** KR107

**Lot Number** 7254

**Date** 22.11.2007


**Expiry Date** 19.11.2008

Reagent	Lot Number
Phos 1	7181
Phos 2	7254
<b>Test Method</b>	LTP 05
<b>Test Instrument</b>	Konelab 20
<b>Serial Number</b>	P4919028

Standard Value	Lot #	Abs.
0		0.002
0.5	P20 08 07	0.141
1	P20 08 07	0.285
1.5	P20 08 07	0.427
2	P20 08 07	0.552

\*serial dilution

Calibration Curve

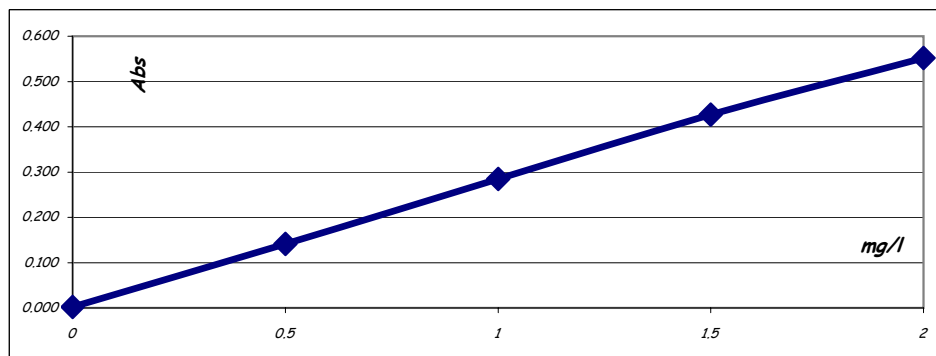

Test	Result	Specification	Pass / Fail
Intercept	0.004	-0.005 to 0.010	Pass
Sensitivity Abs/ppm	0.277	0.260 to 0.320	Pass
Regression	0.999	0.990 to 1.001	Pass

**Notes** Store between 2 & 8 °C  
 \*Stable on Board 5 days  
 Barcode ID = 107  
 \* Based on results obtained in our Research Facility

*Tom Russell.*  
 Dr. T. Russell