

Certificate of Performance

Ammonia 1 Reagent

Product Code KR108
Lot Number 8006

Date 08.01.2007


Expiry Date 02.01.2009

Reagent	Lot Number
AMM 1	8006
Amm 2	7237
Test Method	LTP06
Test Instrument	Konelab 20
Serial Number	P4919028

Std. Value	Lot #	Abs.
0.00		0.018
0.25	AMM 10 10 07	0.215
0.50	AMM 10 10 07	0.411
0.77	AMM 10 10 07	0.625
1.00	AMM 10 10 07	0.801

**serial dilution*

Calibration Curve

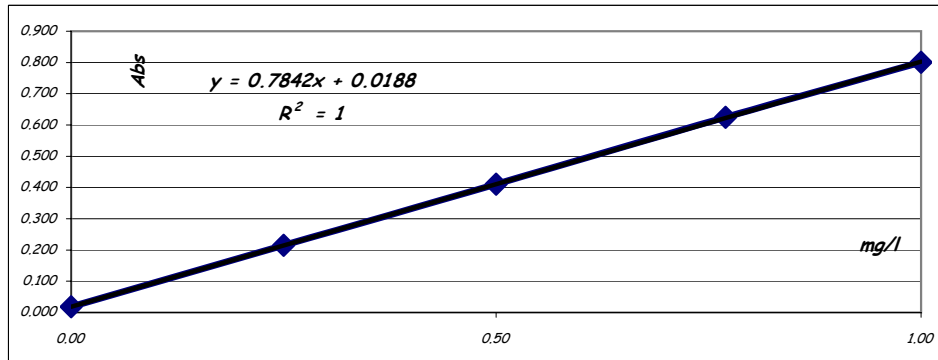

Test	Result	Specification	Pass / Fail
Intercept	0.0188	0.000 to 0.025	Pass
Sensitivity Abs/ppm	0.7842	0.750 to 0.890	Pass
Regression	1.0000	0.990 to 1.0001	Pass

Notes *Store between 2 & 8 °C*
 **Stable on Board 1 day*
 Barcode ID = 108
 ** Based on results obtained in our Research Facility*



Dr. T. Russell