

Certificate of Performance

Ammonia 2 Reagent

Product Code **KR 109**
Lot Number **8022**

Date 05.02.2008


Expiry Date 28.01.2009

Reagent	Lot Number
AMM 1	8021
Amm 2	8022
Test Method	LTP06
Test Instrument	Konelab 20
Serial Number	P4919028

Std. Value	Lot #	Abs.
0.00		0.019
0.25	AMM 10 10 07	0.214
0.50	AMM 10 10 07	0.428
0.77	AMM 10 10 07	0.653
1.00	AMM 10 10 07	0.847

**serial dilution*

Calibration Curve

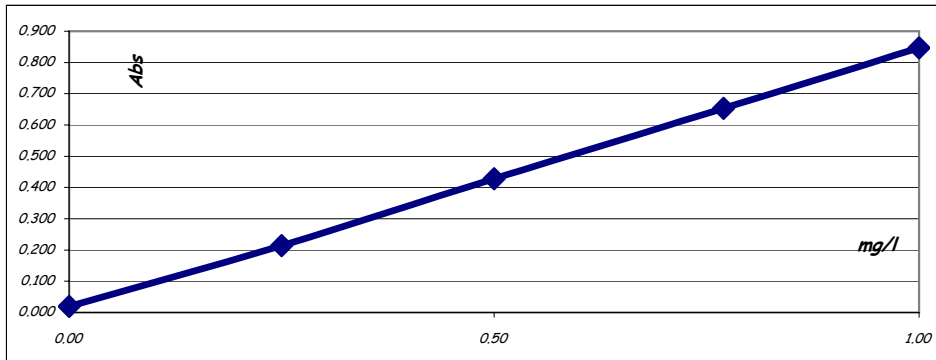

Test	Result	Specification	Pass / Fail
Intercept	0.0132	0.000 to 0.025	Pass
Sensitivity Abs/ppm	0.8313	0.750 to 0.890	Pass
Regression	0.9998	0.990 to 1.0001	Pass

Notes *Store between 2 & 8 °C*
 **Stable on Board 5 days*
 Barcode ID = 109
 ** Based on results obtained in our Research Facility*



Dr. T. Russell