

Certificate of Performance

Phosphate 2 (Phos 2) Reagent

Product Code KR107

Lot Number 8026

Date 06.02.2008


Expiry Date 28.01.2009

Reagent	Lot Number
Phos 1	8019
Phos 2	8026
Test Method	LTP 05
Test Instrument	Konelab 20
Serial Number	P4919028

Standard Value	Lot #	Abs.
0		0.002
0.5	P20 10 07	0.144
1	P20 10 07	0.282
1.5	P20 10 07	0.436
2	P20 10 07	0.561

*serial dilution

Calibration Curve

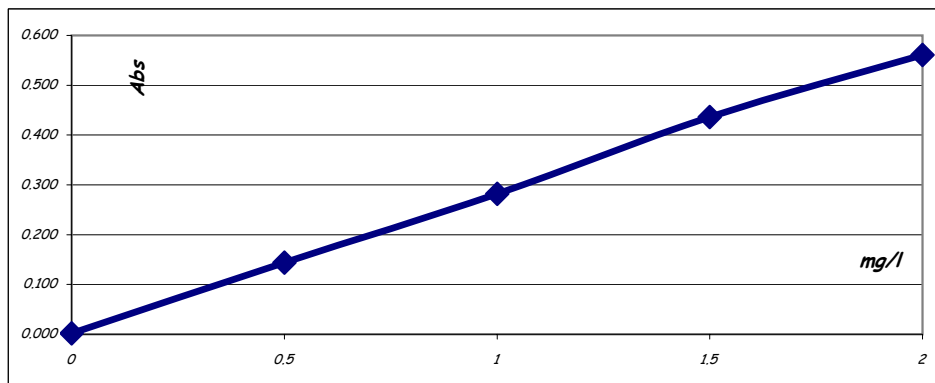

Test	Result	Specification	Pass / Fail
Intercept	0.003	-0.005 to 0.010	Pass
Sensitivity Abs/ppm	0.282	0.260 to 0.320	Pass
Regression	0.999	0.990 to 1.001	Pass

Notes Store between 2 & 8 °C
 *Stable on Board 5 days
 Barcode ID = 107
 * Based on results obtained in our Research Facility

Tom Russell.
 Dr. T. Russell