

Certificate of Performance

**Phosphate 2 (Phos 2) Reagent**

**Product Code** KR107

**Lot Number** 8036

**Date** 03.03.2008


**Expiry Date** 15.02.2009

Reagent	Lot Number
Phos 1	8035
Phos 2	8036
Test Method	LTP 05
Test Instrument	Konelab 20
Serial Number	P4919028

Standard Value	Lot #	Abs.
0		0.003
0.5	P20 10 07	0.150
1	P20 10 07	0.289
1.5	P20 10 07	0.441
2	P20 10 07	0.575

\*serial dilution

**Calibration Curve**

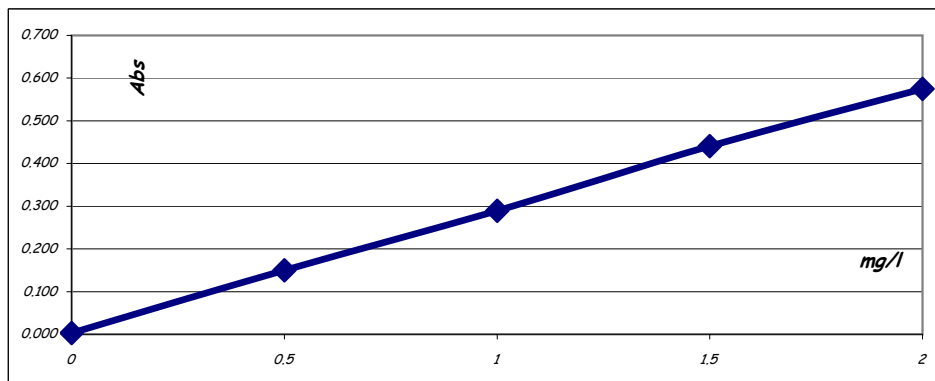

Test	Result	Specification	Pass / Fail
Intercept	0.005	-0.005 to 0.010	Pass
Sensitivity Abs/ppm	0.287	0.260 to 0.320	Pass
Regression	1.000	0.990 to 1.001	Pass

**Notes** Store between 2 & 8 °C  
 \*Stable on Board 5 days  
 Barcode ID = 107  
 \*Based on results obtained in our Research Facility

*Tom Russell.*  
 Dr. T. Russell