

Certificate of Performance

Ammonia 2 Reagent

Product Code **KR 109**
Lot Number **8058**

Date 25.03.2008


Expiry Date 10.03.2009

Reagent	Lot Number
AMM 1	7231
Amm 2	8058
Test Method	LTP06
Test Instrument	Konelab 20
Serial Number	P4919028

Std. Value	Lot #	Abs.
0.00		0.022
0.25	Amm 10 10 07	0.222
0.50	Amm 10 10 07	0.424
0.77	Amm 10 10 07	0.638
1.00	Amm 10 10 07	0.824

**serial dilution*

Calibration Curve

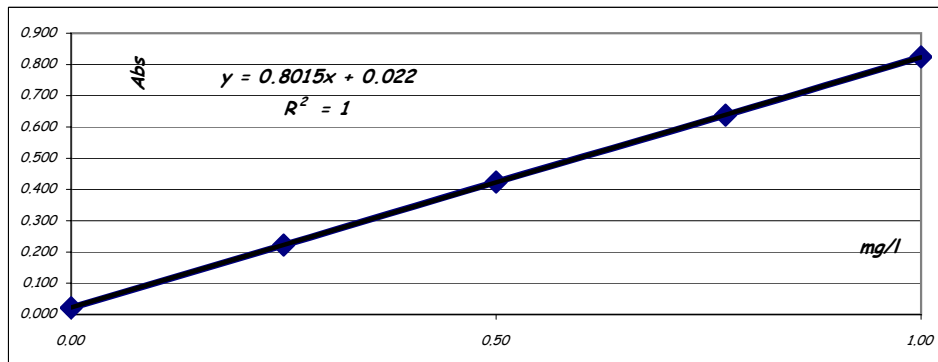

Test	Result	Specification	Pass / Fail
Intercept	0.0220	0.000 to 0.025	Pass
Sensitivity Abs/ppm	0.8015	0.750 to 0.890	Pass
Regression	1.0000	0.990 to 1.0001	Pass

Notes *Store between 2 & 8 °C*

**Stable on Board 5 days*

Barcode ID = 109

** Based on results obtained in our Research Facility*



Dr. T. Russell