

**Certificate of Performance**

**Chloride Reagent**


**Product Code** KR101  
**Lot Number** 8072

**Date** 15.04.2008 **Expiry Date** 09.04.2009

<b>Reagent</b>	<b>Lot Number</b>
Chloride	8072
<b>Test Method</b>	LTP02
<b>Test Instrument</b>	Konelab 20
<b>Serial Number</b>	P4919028

<b>Standard Value</b>	<b>Lot #</b>	<b>Absorbance</b>
0 ppm		0.007
250 ppm	CL25009006	0.323
500 ppm	CL50009006	0.529
800 ppm	CL75009006	0.696
1000 ppm	CL100009006	0.783

**Calibration Curve**

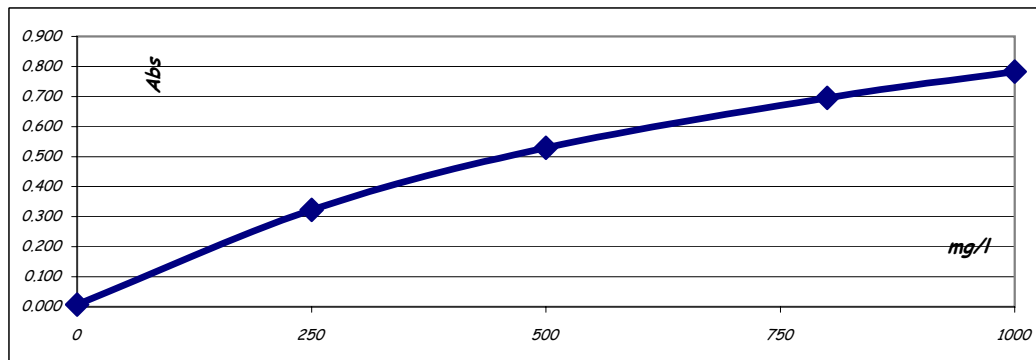

Test	Result	Specification	Pass / Fail
Intercept	0.007	-0.005 to 0.01	<b>Pass</b>
Sensitivity Abs/ppm			
0 - 250 mg/l	0.0013	0.0010 to 0.0016	<b>Pass</b>
250 - 500 mg/l	0.0009	0.0006 to 0.0012	<b>Pass</b>
500 - 800 mg/l	0.0006	0.0004 to 0.0010	<b>Pass</b>
800 - 1000 mg/l	0.0004	0.0003 to 0.0008	<b>Pass</b>

**Notes** Store between 2 & 8 °C  
 \*Stable on Board 5 days  
 Barcode ID = 101  
 \*Based on results obtained in our Research Facility



Dr. T. Russell