

### Certificate of Performance

#### Ammonia 2 Reagent

**Product Code**      **KR 109**  
**Lot Number**        **8075**

**Date**      18.04.2008


**Expiry Date**      09.04.2009

Reagent	Lot Number
AMM 1	8074
Amm 2	8075
<b>Test Method</b>	LTP06
<b>Test Instrument</b>	Konelab 20
<b>Serial Number</b>	P4919028

Std. Value	Lot #	Abs.
0.00		0.018
0.25	AMM 10 03 08	0.215
0.50	AMM 10 03 08	0.419
0.77	AMM 10 03 08	0.633
1.00	AMM 10 03 08	0.813

*\*serial dilution*

#### Calibration Curve

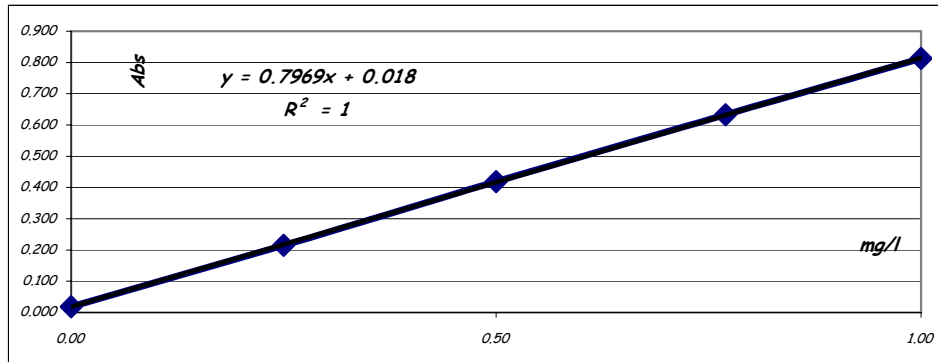

Test	Result	Specification	Pass / Fail
Intercept	0.0180	0.000 to 0.025	<b>Pass</b>
Sensitivity Abs/ppm	0.7969	0.750 to 0.890	<b>Pass</b>
Regression	1.0000	0.990 to 1.0001	<b>Pass</b>

**Notes**      *Store between 2 & 8 °C*  
                  *\*Stable on Board 5 days*  
                  *Barcode ID = 109*  
                  *\* Based on results obtained in our Research Facility*


---

 Dr. T. Russell