Labmedics ANALYTICAL SOLUTIONS

Precision®

'Ready To Use Reagents'

ver 2008.03

Certificate of Performance

Sulphate Reagent

Product Code KR102

Lot Number 8097

Date 22.05.2008 **Expiry Date** 30.04.2009

Reagent	Lot Number
Sulphate	8097
Test Method	LTP01
Test Instrument	Konelab 20
Serial Number	P4919028

Standard Value	Lot #	Abs.
0		0.006
250	Sulp 4000 02 08	0.127
500	Sulp 4000 02 08	0.272
800	Sulp 4000 02 08	0.443
1000	Sulp 4000 02 08	0.559

*serial Dilution

Calibration Curve

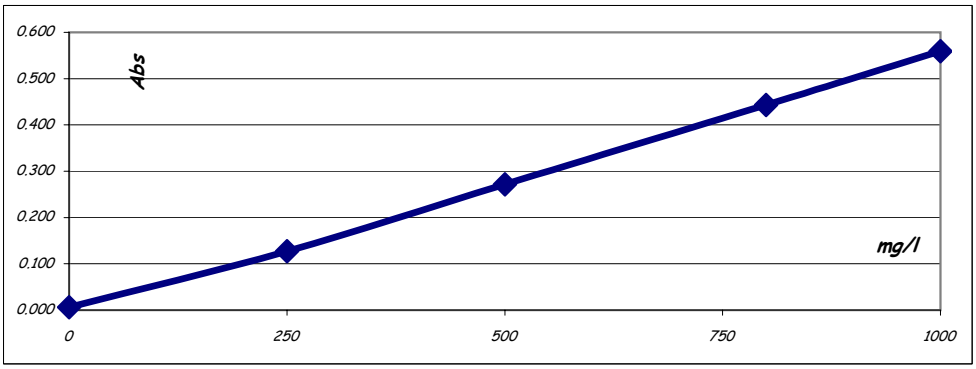

Test		Result	Specification			Pass / Fail
Intercept		0.006	-0.005	to	0.010	Pass
Sensitivity	Abs/ppm					
	0 - 250 mg/l	0.0005	0.0003	to	0.0005	Pass
	250 - 500 mg/l	0.0006	0.0003	to	0.0006	Pass
	500 - 800 mg/l	0.0006	0.0004	to	0.0007	Pass
	800 - 1000 mg/l	0.0006	0.0004	to	0.0008	Pass

Notes *Store between 2 & 8 °C*
**Stable on Board 5 days*
Barcode ID = 102
** Based on results obtained in our Research Facility*

Tom Russell

Dr. T. Russell

Labmedics ANALYTICAL SOLUTIONS
Telegraphic House, Waterfront Quay, Salford Quays, Manchester M50 3XW
Telephone 0161 869 0420