

### Certificate of Performance

#### Ammonia 1 Reagent

**Product Code**      **KR108**  
**Lot Number**        **8159**

**Date**      26.08.2008


**Expiry Date**      22.08.2009

Reagent	Lot Number
AMM 1	<b>8159</b>
Amm 2	8160
<b>Test Method</b>	LTP06
<b>Test Instrument</b>	Konelab 20
<b>Serial Number</b>	P4919028

Std. Value	Lot #	Abs.
0.00		0.022
0.25	AMM 10 03 08	0.220
0.50	AMM 10 03 08	0.424
0.77	AMM 10 03 08	0.641
1.00	AMM 10 03 08	0.831

*\*serial dilution*

#### Calibration Curve

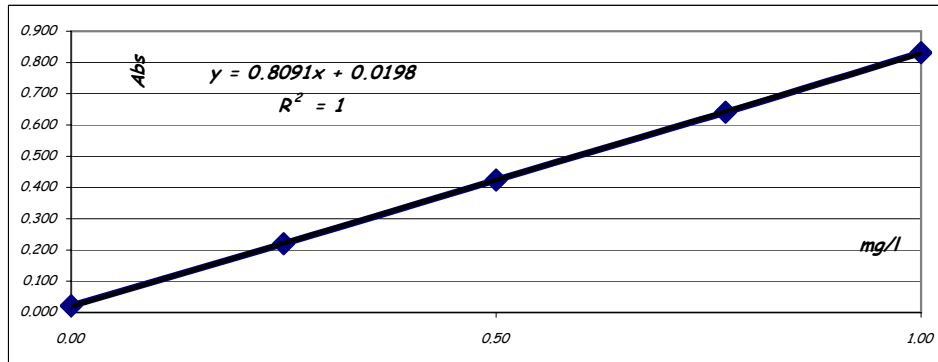

Test	Result	Specification	Pass / Fail
Intercept	0.0198	0.000 to 0.025	<b>Pass</b>
Sensitivity Abs/ppm	0.8091	0.750 to 0.890	<b>Pass</b>
Regression	1.0000	0.990 to 1.0001	<b>Pass</b>

**Notes**      *Store between 2 & 8 °C*

*\*Stable on Board 1 day*

*Barcode ID = 108*

*\* Based on results obtained in our Research Facility*



*Dr. T. Russell*