

Certificate of Performance

Ammonia 2 Reagent

Product Code **KR 109**
Lot Number **8160**

Date 26.08.2008


Expiry Date 22.08.2009

Reagent	Lot Number
AMM 1	8159
Amm 2	8160
Test Method	LTP06
Test Instrument	Konelab 20
Serial Number	P4919028

Std. Value	Lot #	Abs.
0.00		0.022
0.25	AMM 10 03 08	0.220
0.50	AMM 10 03 08	0.424
0.77	AMM 10 03 08	0.641
1.00	AMM 10 03 08	0.831

**serial dilution*

Calibration Curve

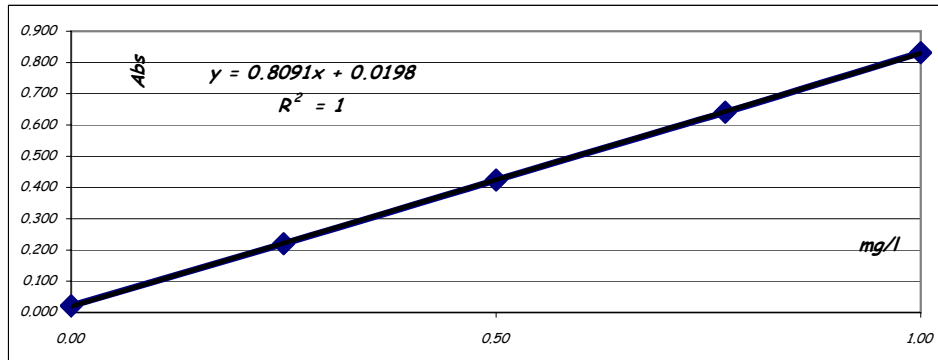

Test	Result	Specification	Pass / Fail
Intercept	0.0198	0.000 to 0.025	Pass
Sensitivity Abs/ppm	0.8091	0.750 to 0.890	Pass
Regression	1.0000	0.990 to 1.0001	Pass

Notes *Store between 2 & 8 °C*
 **Stable on Board 5 days*
 Barcode ID = 109
 ** Based on results obtained in our Research Facility*



 Dr. T. Russell