

Certificate of Performance

**TON 3**

Product Code KR105

Date 17.09.2008


Expiry Date 11.09.2009

Reagent	Lot Number
TON 1	8007
TON 2	8176
TON 3	8177
Test Method	LMTP03
Test Instrument	Konelab 20
Serial Number	P4919028

Std. Value	Lot #	Abs.
0.00		0.002
2.50	TON 100 05 08	0.186
5.00	TON 100 05 08	0.348
7.69	TON 100 05 08	0.521
10.00	TON 100 05 08	0.646

\*serial dilution

Calibration Curve

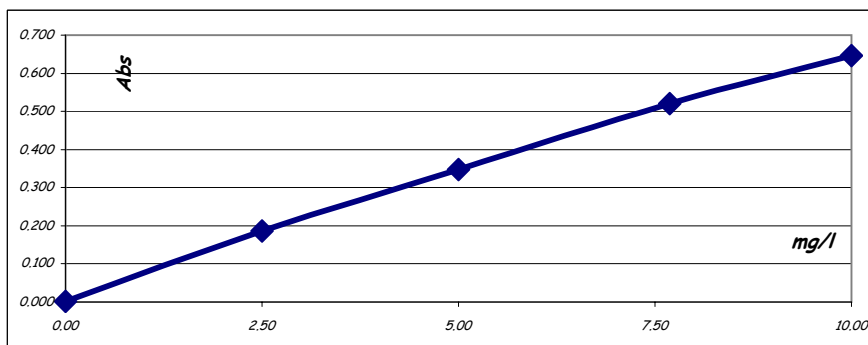

Test	Result	Specification	Pass / Fail
Intercept	0.002	-0.005 to 0.01	Pass
Sensitivity Abs/ppm			
0 - 2.50 mg/l	0.0736	0.0550 to 0.0800	Pass
2.50 - 5.00 mg/l	0.0648	0.0600 to 0.0800	Pass
5.00 - 7.69 mg/l	0.0643	0.0550 to 0.0800	Pass
7.69 - 10.0 mg/l	0.0541	0.0500 to 0.0700	Pass

**Notes** Store between 2 & 8 °C  
 \*Stable on Board TON 1 - 1 day  
                                   \* TON 2 & TON 3 - 5 days:  
 Keep Tightly Sealed when not in use.  
 Do not return unused portions to container  
 Barcode ID- TON 1 103; TON 2 104; TON 3 105  
 \* Based on results obtained in our Research Facility



Dr. T. Russell