

**Certificate of Performance**
**Phosphate 2 (Phos 2) Reagent**
**Product Code** KR107

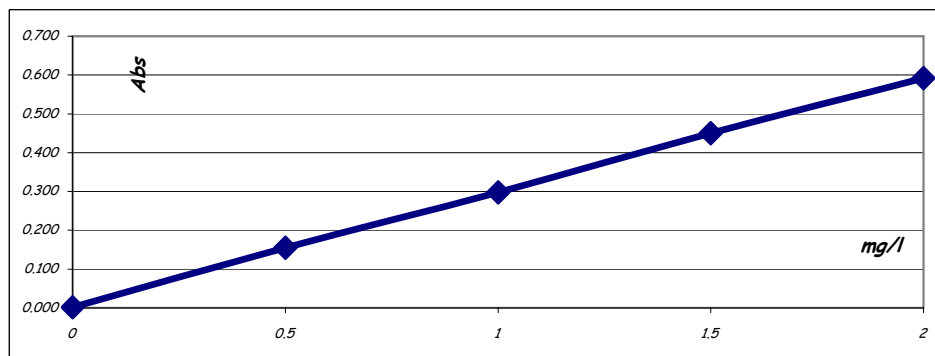
**Lot Number** 8179

**Date** 19.09.2008

**Expiry Date** 11.09.2009

Reagent	Lot Number
Phos 1	8178
Phos 2	8179
<b>Test Method</b>	LTP 05
<b>Test Instrument</b>	Konelab 20
<b>Serial Number</b>	P4919028

Standard Value	Lot #	Abs.
0		0.002
0.5	P20 02 08	0.155
1	P20 02 08	0.298
1.5	P20 02 08	0.450
2	P20 02 08	0.592

*\*serial dilution*
**Calibration Curve**


Test	Result	Specification	Pass / Fail
Intercept	0.004	-0.005 to 0.010	<b>Pass</b>
Sensitivity Abs/ppm	0.295	0.260 to 0.320	<b>Pass</b>
Regression	1.000	0.990 to 1.001	<b>Pass</b>

Notes Store between 2 & 8 °C  
 \*Stable on Board 5 days  
 Barcode ID = 107  
 \* Based on results obtained in our Research Facility

  
 Dr. T. Russell