

Certificate of Performance

Phosphate 2 (Phos 2) Reagent

Product Code KR107
Lot Number 8225

Date 14.11.2008


Expiry Date 14.11.2009

Reagent	Lot Number
Phos 1	8042
Phos 2	8225
Test Method	LTP 05
Test Instrument	Konelab 20
Serial Number	P4919028

Standard Value	Lot #	Abs.
0		0.003
0.5	P20 09 08	0.153
1	P20 09 08	0.290
1.5	P20 09 08	0.445
2	P20 09 08	0.583

*serial dilution

Calibration Curve

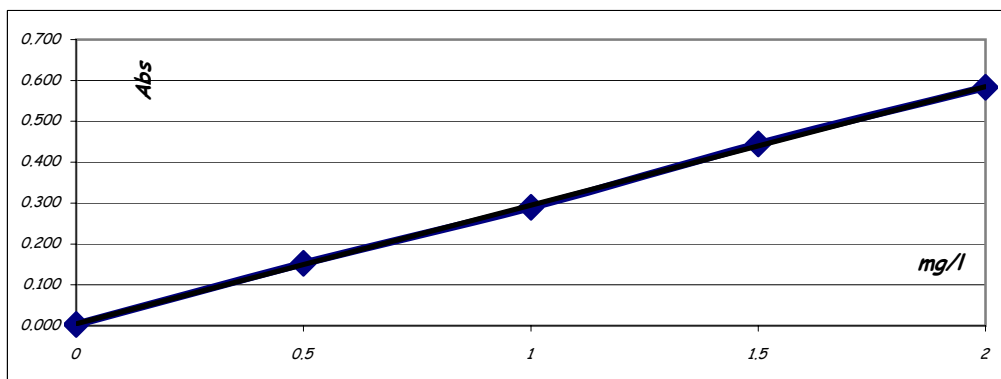

Test	Result	Specification	Pass / Fail
Intercept	0.004	-0.005 to 0.010	Pass
Sensitivity Abs/ppm	0.290	0.260 to 0.320	Pass
Regression	1.000	0.990 to 1.001	Pass

Notes Store between 2 & 8 °C
*Stable on Board 5 days
Barcode ID = 107
* Based on results obtained in our Research Facility

Tom Russell.
Dr. T. Russell