

Certificate of Performance
Phosphate 1 (Phos 1) Reagent
Product Code KR106

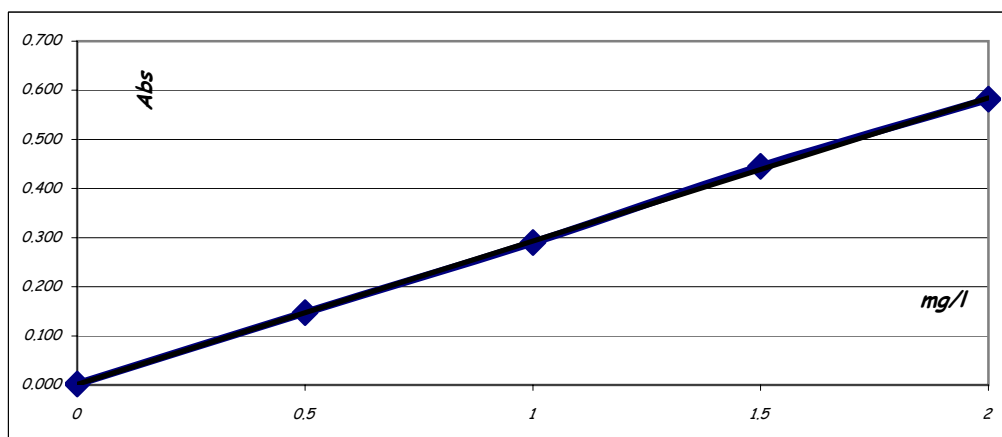
Lot Number 8228

Date 20.11.2008

Expiry Date 14.11.2009

Reagent	Lot Number
Phos 1	8228
Phos 2	8215
Test Method	LTP 05
Test Instrument	Konelab 20
Serial Number	P4919028

Standard Value	Lot #	Abs.
0		0.002
0.5	P20 08 08	0.147
1	P20 08 08	0.290
1.5	P20 08 08	0.445
2	P20 08 08	0.582

**serial dilution*
Calibration Curve


	Result	Specification	Pass / Fail
Intercept	0.002	-0.005 to 0.010	Pass
Sensitivity Abs/ppm	0.292	0.260 to 0.320	Pass
Regression	1.000	0.990 to 1.001	Pass

Notes Store between 2 & 8 °C
 *Stable on Board 5 days
 Barcode ID = 106
 * Based on results obtained in our Research Facility



Dr. T. Russell