

Certificate of Performance

Sulphate Reagent

Product Code KR102
Lot Number 8231


Date 19.11.2008 **Expiry Date** 10.11.2009

Reagent	Lot Number
Sulphate	8231
Test Method	LTP01
Test Instrument	Konelab 20
Serial Number	P4919028

Standard Value	Lot #	Abs.
0		0.005
250	Sulp 4000 08 08	0.125
500	Sulp 4000 08 08	0.271
800	Sulp 4000 08 08	0.445
1000	Sulp 4000 08 08	0.549

*serial Dilution

Calibration Curve

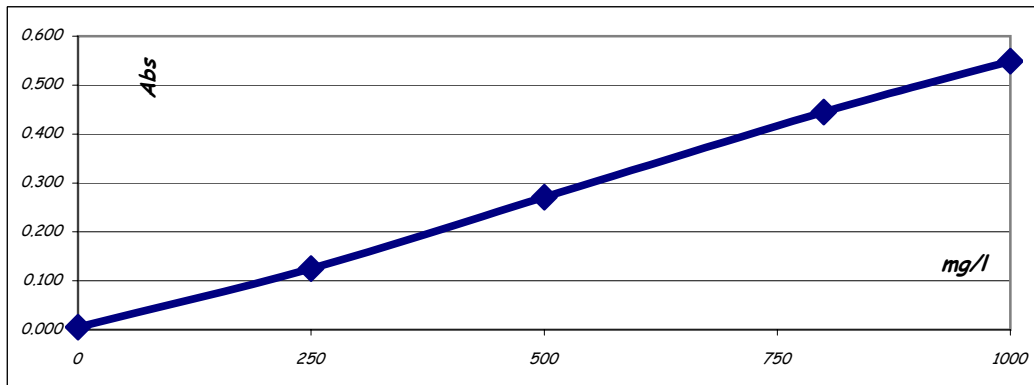

Test	Result	Specification	Pass / Fail
Intercept	0.005	-0.005 to 0.010	Pass
Sensitivity Abs/ppm			
0 - 250 mg/l	0.0005	0.0003 to 0.0005	Pass
250 - 500 mg/l	0.0006	0.0003 to 0.0006	Pass
500 - 800 mg/l	0.0006	0.0004 to 0.0007	Pass
800 - 1000 mg/l	0.0005	0.0004 to 0.0008	Pass

Notes Store between 2 & 8 °C
*Stable on Board 5 days
Barcode ID = 102
* Based on results obtained in our Research Facility

Tom Russell

Dr. T. Russell