

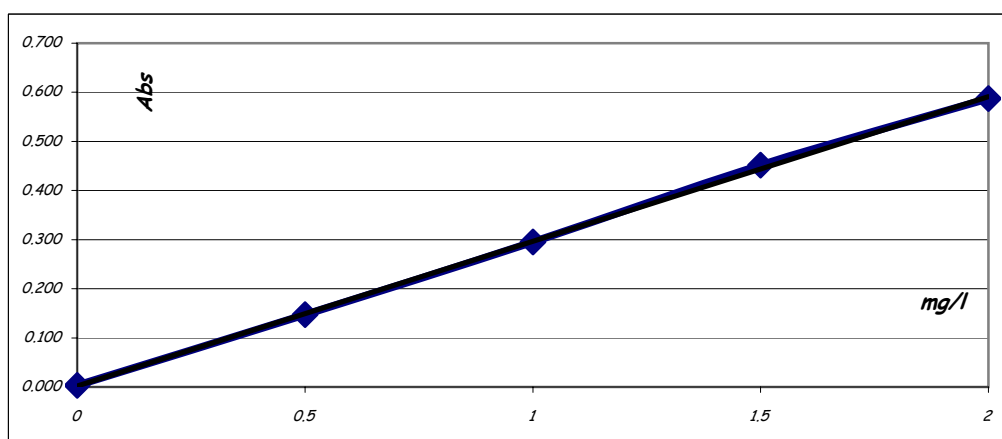
**Certificate of Performance**
**Phosphate 1 (Phos 1) Reagent**
**Product Code** KR106  
**Lot Number** 9010

**Date** 23.01.2009

**Expiry Date** 02.01.2010

Reagent	Lot Number
Phos 1	9010
Phos 2	8105
<b>Test Method</b>	LTP 05
<b>Test Instrument</b>	Konelab 20
<b>Serial Number</b>	P4919028

Standard Value	Lot #	Abs.
0		0.003
0.5	P20 09 08	0.147
1	P20 09 08	0.295
1.5	P20 09 08	0.452
2	P20 09 08	0.587

*\*serial dilution*
**Calibration Curve**


	Result	Specification	Pass / Fail
Intercept	0.002	-0.005 to 0.010	<b>Pass</b>
Sensitivity Abs/ppm	0.295	0.260 to 0.320	<b>Pass</b>
Regression	1.000	0.990 to 1.001	<b>Pass</b>

**Notes** Store between 2 & 8 °C  
 \*Stable on Board 5 days  
 Barcode ID = 106  
 \* Based on results obtained in our Research Facility



Dr. T. Russell