

**Certificate of Performance**
**Ammonia 1 Reagent**

**Product Code** KR108  
**Lot Number** 9031

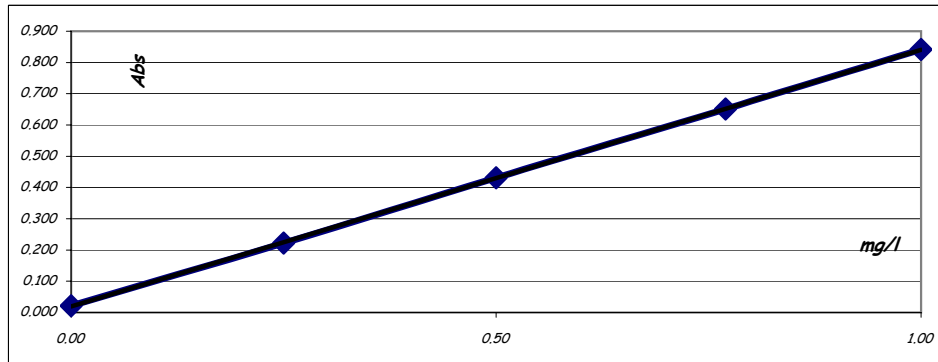
**Date** 02.02.2009

**Expiry Date** 30.01.2010

Reagent	Lot Number
AMM 1	9031
Amm 2	9032
<b>Test Method</b>	LTP06
<b>Test Instrument</b>	Konelab 20
<b>Serial Number</b>	P4919028

Std. Value	Lot #	Abs.
0.00		0.022
0.25	AMM 10 09 08	0.222
0.50	AMM 10 09 08	0.431
0.77	AMM 10 09 08	0.651
1.00	AMM 10 09 08	0.842

*\*serial dilution*

**Calibration Curve**


Test	Result	Specification	Pass / Fail
Intercept	0.0198	0.000 to 0.025	<b>Pass</b>
Sensitivity Abs/ppm	0.8210	0.750 to 0.890	<b>Pass</b>
Regression	1.0000	0.990 to 1.0001	<b>Pass</b>

**Notes** Store between 2 & 8 °C

\*Stable on Board 1 day

Barcode ID = 108

\* Based on results obtained in our Research Facility



Dr. T. Russell